



## testo 350 · Flue gas analyzer

Instruction manual



---

# 1 Contents

<b>1</b>	<b>Contents .....</b>	<b>3</b>
<b>2</b>	<b>Safety and the environment .....</b>	<b>7</b>
2.1.	About this document .....	7
2.2.	Ensure safety .....	8
2.3.	Product-specific safety instructions .....	10
2.4.	Protecting the environment.....	10
<b>3</b>	<b>Specifications .....</b>	<b>11</b>
3.1.	Use.....	11
3.2.	Technical data .....	11
3.2.1.	Examinations and licenses .....	11
3.2.2.	Bluetooth® module (option).....	11
3.2.3.	Declaration of Conformity .....	14
3.2.4.	Measurement ranges and resolution .....	14
3.2.5.	Accuracy and response time.....	15
3.2.6.	Measurement range extension for individual slot (option).....	17
3.2.7.	Fresh air valve (option) .....	18
3.2.8.	Other instrument data.....	19
<b>4</b>	<b>Product description .....</b>	<b>21</b>
4.1.	Control Unit.....	21
4.1.1.	Overview .....	21
4.1.2.	Keyboard .....	22
4.1.3.	Display .....	23
4.1.4.	Connections / interfaces.....	24
4.1.5.	Menu guidance for control unit .....	24
4.2.	Meas. box .....	26
4.2.1.	Overview .....	26
4.2.2.	Status display.....	27
4.2.3.	Connections / interfaces.....	28
4.2.4.	Functions / instrument options .....	28
4.2.5.	Menu guidance meas. box.....	29
4.2.6.	Modular flue gas probe .....	31
<b>5</b>	<b>First steps .....</b>	<b>32</b>
5.1.	Commissioning.....	32

5.2.	Getting to know the product .....	32
5.2.1.	Mains unit, batteries/rechargeable batteries .....	32
5.2.1.1.	Recharging the rech. batt. of the Control Unit .....	32
5.2.1.2.	Charging the rech. batt. of the meas. box .....	33
5.2.1.3.	Battery care .....	33
5.2.1.4.	Mains operation.....	33
5.2.2.	Connecting probes / sensors.....	34
5.2.3.	Occupying the trigger input .....	34
5.2.4.	Connecting system components .....	36
5.2.4.1.	Connection using contact strip.....	36
5.2.4.2.	Connection using a Data bus cable (accessory part to a bus system) .....	36
5.2.4.3.	Connection via Bluetooth® (option).....	39
5.2.5.	Switching on .....	40
5.2.6.	Calling up a function .....	41
5.2.7.	Entering values .....	41
5.2.8.	Printing / saving data .....	42
5.2.9.	Search for meas. boxes .....	43
5.2.10.	Confirming an error message.....	43
5.2.11.	Switching off.....	43
5.3.	Folders / Locations.....	44
5.4.	Measurement records .....	46
5.5.	Instrument diagnosis.....	48
5.5.1.	Error diagnosis .....	48
5.5.2.	Gas path check.....	48
5.5.3.	Sensor diagnosis .....	48
5.5.4.	Instrument information .....	49
6	Using the product.....	50
6.1.	Performing settings.....	50
6.1.1.	Assigning the right hand function key .....	50
6.1.2.	Instrument settings.....	50
6.1.2.1.	Dilution .....	50
6.1.2.2.	Measurement view .....	52
6.1.2.3.	Units.....	54
6.1.2.4.	Date / time .....	55
6.1.2.5.	Power options.....	55
6.1.2.6.	Display brightness.....	55
6.1.2.7.	Printer .....	55
6.1.2.8.	Bluetooth® .....	56
6.1.2.9.	Language.....	57
6.1.2.10.	Country version.....	57
6.1.2.11.	Password protection .....	58

---

6.1.2.12.	Analog input .....	58
6.1.2.13.	Data bus.....	59
6.1.3.	Fuels .....	59
6.1.4.	Sensor settings .....	60
6.1.4.1.	NO <sub>2</sub> addition .....	60
6.1.4.2.	CxHy-Sensor.....	60
6.1.4.3.	Sensor protection .....	61
6.1.4.4.	Calibration / adjustment .....	61
6.1.4.5.	ppmh counter .....	64
6.1.4.6.	Calibration data .....	65
6.1.4.7.	Adjustment data .....	65
6.1.4.8.	Negative value .....	65
6.1.5.	Programs .....	66
<b>6.2.</b>	<b>Measuring .....</b>	<b>69</b>
6.2.1.	Preparing for measurement.....	69
6.2.2.	Using the flue gas probe .....	71
6.2.3.	Applications.....	71
6.2.3.1.	Flue Gas, Flue Gas + m/s, Flue Gas + $\Delta p$ , Program for all meas. boxes, Flue Gas before + after catalyst .....	73
6.2.3.2.	Draught-Measurement .....	75
6.2.3.3.	Smoke number/HCT.....	76
6.2.3.4.	Gas rating.....	76
6.2.3.5.	Oil flow rate .....	77
<b>6.3.</b>	<b>Analog outputs.....</b>	<b>77</b>
<b>7</b>	<b>Maintaining the product.....</b>	<b>80</b>
7.1.	Changing the rechargeable battery .....	80
7.2.	Cleaning the flue gas analyser.....	80
7.3.	Changing / retrofitting sensors .....	81
7.4.	Replacing the filter for NO sensors .....	84
7.5.	Recalibrating sensors .....	84
7.6.	Cleaning the modular flue gas probe .....	85
7.7.	Replacing probe pre-filter .....	85
7.8.	Changing the thermocouple .....	85
7.9.	Condensate trap / condensate container .....	86
7.10.	Checking / replacing the dirt filter .....	87
7.11.	Cleaning / replacing the pump.....	88

# 1 Contents

---

7.11.1. Cleaning the main gas pump.....	89
7.11.2. Changing the main gas pump.....	90
7.11.3. Changing the condensate pump .....	90
7.11.4. Replacing the motor of the condensate pump.....	91
7.12. Replacing the filtration non-woven in the gas cooler.....	93
7.13. Recommended maintenance cycles .....	94
<b>8 Tips and assistance .....</b>	<b>95</b>
8.1. Questions and answers.....	95
8.2. Accessories and spare parts.....	96
8.3. Updating the instrument software .....	100
<b>9 Appendix.....</b>	<b>102</b>

## 2 Safety and the environment

### 2.1. About this document



This document describes the product testo 350 with the device setting **Country version** | **Great Britain**.

#### Use


- > Please read this documentation through carefully and familiarize yourself with the product before putting it to use. Pay particular attention to the safety instructions and warning advice in order to prevent injuries and damage to the products.
- > Keep this document to hand so that you can refer to it when necessary.
- > Hand this documentation on to any subsequent users of the product.

#### Warnings

Always pay attention to information that is marked by the following warnings with warning pictograms. Implement the specified precautionary measures.

Representation	Explanation
 <b>WARNING</b>	Indicates potential serious injuries
 <b>CAUTION</b>	indicates potential minor injuries
<b>NOTICE</b>	indicates circumstances that may lead to damage to the products

#### Symbols and writing standards


	Explanation
	Note: Basic or further information.
1. ... 2. ...	Action: more steps, the sequence must be followed.
> ...	Action: a step or an optional step.
- ...	Result of an action.

<b>Menu</b>	Elements of the instrument, the instrument displays or the program interface.
<b>[OK]</b>	Control keys of the instrument or buttons of the program interface.
...   ...	Functions/paths within a menu.
“...”	Example entries

### 2.2. Ensure safety

- > Only operate the product properly, for its intended purpose and within the parameters specified in the technical data. Do not use any force.
- > Do not operate the instrument if there are signs of damage at the housing, mains unit or feed lines.
- > Do not perform contact measurements on non-insulated, live parts.
- > Do not store the product together with solvents. Do not use any desiccants.
- > Carry out only the maintenance and repair work on this instrument that is described in the documentation. Follow the prescribed steps exactly. Use only original spare parts from Testo.
- > Any further or additional work must only be carried out by authorised personnel. Testo will otherwise refuse to accept responsibility for the proper functioning of the measuring instrument after repair and for the validity of certifications.
- > Only use the device in closed, dry rooms and protect it from rain and moisture.
- > Temperatures given on probes/sensors relate only to the measuring range of the sensors. Do not expose handles and feed lines to any temperatures in excess of 70 °C unless they are expressly permitted for higher temperatures.
- > Dangers may also arise from the systems being measured or the measuring environment: Note the safety regulations valid in your area when performing the measurements.

**Safety related symbols on the instrument**

Representation	Explanation
	<p>If the product is not used in strict compliance with this documentation, the intended protection may be impaired.</p> <ul style="list-style-type: none"> <li>&gt; Operate the product only as described in this documentation.</li> <li>&gt; Please consult your dealer or the manufacturer if in doubt.</li> </ul>

- > When carrying out any measurement, please observe the relevant lower explosion limit (LEL) of carbon monoxide, methane, propane, butane, etc.
  - Observe the lower explosive limit when measuring CO:  
LEL = 12.5 % (125,000 ppm)
  - Observe the lower explosive limit when measuring HC:  
LEL of natural gas: 5.0 % (50,000 ppm)  
LEL of propane: 21.0 % (21,000 ppm)  
LEL of butane: 1.5 % (18,000 ppm)

**For products with Bluetooth® (optional)**

Changes or modifications that have been made without the explicit consent of the responsible approval authority may cause cancellation of the type approval.

Data transfer may be disturbed by equipment that uses the same ISM band, e.g. WLAN, microwave ovens, ZigBee.

The use of radio communication links is not permitted in aeroplanes and hospitals, among other locations. For this reason the following points must be ensured before entering:

- > Switch off the instrument (control unit and analyzer box).
- > Disconnect control unit and analyzer box from all external power sources (mains cable, external rechargeable batteries, etc.).

## 2.3. Product-specific safety instructions

### CAUTION

Acid in the sensors.

#### **May cause chemical burns.**

- > Do not open the sensors.  
Eye contact: Rinse the affected eye thoroughly under running water for 10 minutes, keeping the eyelids wide open and protecting the unaffected eye. Remove contact lenses wherever possible.

### CAUTION

Acid in the sensor filters.

#### **May cause irritation to the skin, eyes or respiratory tract.**

- > Do not open the sensor filters.  
Eye contact: Rinse the affected eye thoroughly under running water for 10 minutes, keeping the eyelids wide open and protecting the unaffected eye. Remove contact lenses wherever possible.  
Skin contact: Remove the injured person's contaminated clothing, ensuring self-protection. Rinse affected skin areas under running water for at least 10 minutes.  
Inhalation: Move to fresh air and make sure that breathing is unrestricted.  
Ingestion: Rinse mouth out and spit out liquid. If conscious, drink 1 glass of water (approx. 200 ml). Do not induce vomiting.

## 2.4. Protecting the environment

- > Dispose of faulty rechargeable batteries/spent batteries in accordance with the valid legal specifications.
- > At the end of its useful life, send the product to the separate collection for electric and electronic devices (observe local regulations) or return the product to Testo for disposal.

## 3 Specifications

### 3.1. Use

The testo 350 is a portable flue gas analyser for professional flue gas analysis. The instrument consists of the Control Unit (control unit for displaying readings and controlling the meas. box) and the meas. box (measuring instrument). Plug-type contacts, databus cable or Bluetooth® (option) are used to connect the Control Unit to the meas. box.

The testo 350 has been designed for the following tasks / applications:

- Service / adjustment of industrial furnace systems (processing plants, power plants)
- Emission control and inspection of compliance with emission guidelines
- Service / commissioning of burners / boilers in industrial areas
- Measurements on gas turbines / stationary industrial engines

testo 350 must not be used:

- for continuous measurements
- as a safety (alarm) device
- to measure combustion gases (before the actual combustion process)

### 3.2. Technical data

#### 3.2.1. Examinations and licenses

As declared in the certificate of conformity, this product complies with Directive 2014/30/EC.

This product is TÜV approved.

#### 3.2.2. Bluetooth® module (option)

---








The use of the wireless module is subject to the regulations and stipulations of the respective country of use, and the module may only be used in each case in countries for which a country certification has been granted.

The user and every owner undertake to adhere to these regulations and prerequisites for use, and acknowledge that the re-sale, export, import, etc. in particular in, to or from countries without wireless permits, is their responsibility.

---

### 3 Specifications

Product	testo 350 Analyse box Control Unit
Mat.-No.	0632 3510 0632 3511
Date	17.09.2020
<b>Country</b>	<b>Comments</b>
Canada	contains IC 5123A-WT11U IC Warnings
Europa + EFTA (Länderliste einfügen)	 <b>EU countries:</b> Belgium (BE), Bulgaria (BG), Denmark (DK), Germany (DE), Estonia (EE), Finland (FI), France (FR), Greece (GR), Ireland (IE), Italy (IT), Latvia (LV), Lithuania (LT), Luxembourg (LU), Malta (MT), Netherlands (NL), Austria (AT), Poland (PL), Portugal (PT), Romania (RO), Sweden (SE), Slovakia (SK), Slovenia (SI), Spain (ES), Czech Republic (CZ), Hungary (HU), United Kingdom (GB), Republic of Cyprus (CY).  <b>EFTA countries:</b> Iceland, Liechtenstein, Norway, Switzerland
Japan	  <b>209- J00232</b> Japan Information
Malaysia	Authorized
South Korea	 Analyse box: R-R-TTT-testo350KB    Control Unit: R-R-TTT-testo350KR  see KCC Warning

USA	 contains FCC ID: QQQWT11U FCC Warnings																			
Radio module	<table border="1"> <thead> <tr> <th data-bbox="423 316 647 338">Feature</th> <th data-bbox="647 316 893 338">Values</th> </tr> </thead> <tbody> <tr> <td data-bbox="423 338 647 360">Bluetooth Range</td> <td data-bbox="647 338 893 360">&lt;10 m (free field)</td> </tr> <tr> <td data-bbox="423 360 647 405">Bluetooth type</td> <td data-bbox="647 360 893 405">Bluegiga WTT11u Bluetooth Module</td> </tr> <tr> <td data-bbox="423 405 647 427">Qualified Design ID</td> <td data-bbox="647 405 893 427">22298</td> </tr> <tr> <td data-bbox="423 427 647 450">Declaration ID</td> <td data-bbox="647 427 893 450">B016141</td> </tr> <tr> <td data-bbox="423 450 647 472">Bluetooth radio class</td> <td data-bbox="647 450 893 472">Class 1</td> </tr> <tr> <td data-bbox="423 472 647 494">Bluetooth company</td> <td data-bbox="647 472 893 494">Silicon Laboratories Inc.</td> </tr> <tr> <td data-bbox="423 494 647 517">RF Band</td> <td data-bbox="647 494 893 517">2402 - 2480 MHz</td> </tr> <tr> <td data-bbox="423 517 647 539">Nominal output power</td> <td data-bbox="647 517 893 539">17 dBm</td> </tr> </tbody> </table>		Feature	Values	Bluetooth Range	<10 m (free field)	Bluetooth type	Bluegiga WTT11u Bluetooth Module	Qualified Design ID	22298	Declaration ID	B016141	Bluetooth radio class	Class 1	Bluetooth company	Silicon Laboratories Inc.	RF Band	2402 - 2480 MHz	Nominal output power	17 dBm
Feature	Values																			
Bluetooth Range	<10 m (free field)																			
Bluetooth type	Bluegiga WTT11u Bluetooth Module																			
Qualified Design ID	22298																			
Declaration ID	B016141																			
Bluetooth radio class	Class 1																			
Bluetooth company	Silicon Laboratories Inc.																			
RF Band	2402 - 2480 MHz																			
Nominal output power	17 dBm																			

## IC Warnings

### RSS-Gen & RSS-247 statement:

This device complies with Industry Canada licence-exempt RSS standard(s). Operation is subject to the following two conditions:

- (1) this device may not cause interference, and
- (2) this device must accept any interference, including interference that may cause undesired operation of the device.

Le présent appareil est conforme aux CNR d'Industrie Canada applicables aux appareils radio exempts de licence.

L'exploitation est autorisée aux deux conditions suivantes :

- (1) l'appareil ne doit pas produire de brouillage, et
- (2) l'utilisateur de l'appareil doit accepter tout brouillage radioélectrique subi, même si le brouillage est susceptible d'en compromettre le fonctionnement.

## FCC Warnings

Information from the FCC (Federal Communications Commission)

### For your own safety

Shielded cables should be used for a composite interface. This is to ensure continued protection against radio frequency interference.

### FCC warning statement

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

## 3 Specifications

---

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

### Caution

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment. Shielded interface cable must be used in order to comply with the emission limits.

### Warning

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions:

- (1) this device may not cause harmful interference, and
- (2) this device must accept any interference received, including interference that may cause undesired operation.

## Japan Information

当該機器には電波法に基づく、技術基準適合証明等を受けた特定無線設備を装着している。

## KCC Warning

해당 무선 설비는 운용 중 전파혼신 가능성이 있음.

### 3.2.3. Declaration of Conformity

---



You can find the EU declaration of conformity on the Testo website [www.testo.com](http://www.testo.com) under the product-specific downloads.

---

### 3.2.4. Measurement ranges and resolution

#### Analysis box

Measurement parameter	Measurement range	Resolution
O <sub>2</sub>	0...25vol.%	0.01vol.%
CO, H <sub>2</sub> -comp.	0...10000ppm	1ppm
CO <sub>low</sub> , H <sub>2</sub> -comp.	0...500ppm	0.1ppm
NO	0...4000ppm	1ppm
NO <sub>low</sub>	0...300ppm	0.1ppm

Measurement parameter	Measurement range	Resolution
NO <sub>2</sub>	0...500ppm	0.1ppm
SO <sub>2</sub>	0...500ppm	1ppm
H <sub>2</sub> S	0...300ppm	0.1ppm
CO <sub>2</sub> -(IR)	0...50vol.%	0.01Vol.% (0...25Vol.%) 0.1Vol.% (> 25Vol.%)
CxHy <sup>1, 2</sup>	Natural gas: 100...40000ppm Propane: 100...21000ppm Butane: 100...18000ppm	10ppm 10ppm 10ppm
Differential pressure 1	-40...40hPa	0.01hPa
Differential pressure 2	-200...200hPa	0.1hPa
NTC (permanently installed)	-20 to 50°C	0.1°C
Abs. Press., optionally when IR sensor is installed	600...1150hPa	1hPa
Flow velocity	0...40m/s	0.1m/s
Type K (NiCr-Ni)	-200 to 1370°C	0.1°C
Type S (Pt10Rh-Pt)	0 to 1760°C	0,1°C

### 3.2.5. Accuracy and response time

#### Analysis box

Measurement parameter	Accuracy	Response time
O <sub>2</sub>	±0.2Vol.%	< 20s (t95)

<sup>1</sup> Detection limit: 50ppm

<sup>2</sup> Strict compliance with the lower explosion limit is mandatory.

### 3 Specifications

Measurement parameter	Accuracy	Response time
CO, H <sub>2</sub> -comp.	±10ppm (0...199ppm) ±5% of reading (200...2000ppm) ±10% of reading (rest of range)	< 40s (t <sub>90</sub> )
CO <sub>low</sub> , H <sub>2</sub> -comp.	±2ppm (0...39.9ppm CO) ±5% of reading (rest of range)	< 40s (t <sub>90</sub> )
NO	±5ppm (0...99ppm) ±5% of reading (100...1999.9ppm) ±10% of reading (rest of range)	< 30s (t <sub>90</sub> )
NO <sub>low</sub>	±2ppm (0...39.9ppm) ±5% of reading (rest of range)	< 30s (t <sub>90</sub> )
NO <sub>2</sub>	±5ppm (0...99.9ppm) ±5% of reading (rest of range)	< 40s (t <sub>90</sub> )
SO <sub>2</sub>	±5ppm (0...99ppm) ±5% of reading (100...1999ppm) ±10% of reading (rest of range)	< 30s (t <sub>90</sub> )
H <sub>2</sub> S	±2ppm (0...39.9ppm) ±5% of reading (rest of range)	< 35s (t <sub>90</sub> )
CO <sub>2</sub> -(IR)	±0.3Vol.% ±1% of reading (0...25Vol.%) ±0.5Vol.% ±1.5% of reading (rest of range)	< 10s (t <sub>90</sub> ) heat-up time: < 15min
CxHy	±400ppm (100...4000ppm) ±10% of reading (rest of range)	< 40s (t <sub>90</sub> )
Differential pressure 1	±0.03hPa (-2.99...2.99hPa) ±1.5% of reading (rest of range)	-
Differential pressure 2	±0.5hPa (-49.9...49.9hPa) ±1.5% of reading (rest of range)	-
Absolute pressure	±10hPa	-
Type K (NiCr-Ni)	±0.4°C (-100 to 200°C) ±1°C (rest of range)	-
Type S (Pt10Rh-Pt)	±1°C (0 to 1760°C)	-

Measurement parameter	Accuracy	Response time
Combustion air (VT) via permanently installed NTC	$\pm 0.2^{\circ}\text{C}$ (-10...50 $^{\circ}\text{C}$ ) $\pm 3^{\circ}\text{C}$ Offset	-

### 3.2.6. Measurement range extension for individual slot (option)

Measurement parameter	Max. measuring range with highest dilution factor 40	Accuracy <sup>3</sup>	Resolution
CO, H <sub>2</sub> -comp.	0...400000ppm	$\pm 2\%$ of reading	1 ppm
CO <sub>low</sub> , H <sub>2</sub> -comp.	0...20000ppm	$\pm 2\%$ of reading	0.1 ppm
SO <sub>2</sub>	0...200000ppm	$\pm 2\%$ of reading	1 ppm
NO <sub>low</sub>	0...12000ppm	$\pm 2\%$ of reading	0.1 ppm
NO	0...160000ppm	$\pm 2\%$ of reading	1 ppm
CxHy <sup>4, 5</sup>	Natural gas: 100...40000ppm Propane: 100...21000ppm Butane: 100...18000ppm	$\pm 2\%$ of reading	10 ppm 10 ppm 10 ppm

Dilution stages: x2, x5, x10, x20, x40

<sup>3</sup> The additional measuring inaccuracy, that needs to be added to the measuring inaccuracy without dilution, is specified.

<sup>4</sup> Detection limit: 50ppm

<sup>5</sup> Strict compliance with the lower explosion limit is mandatory.

### 3.2.7. Fresh air valve (option)

Dilution of all sensors, dilution factor 5

Measurement parameter	Measurement range	Accuracy <sup>6, 7</sup>
O <sub>2</sub>	The reading does not appear in the display.	-
CO, H <sub>2</sub> -comp.	2500...50000ppm	±5% of reading (-150...0hPa)
CO <sub>low</sub> , H <sub>2</sub> -comp.	500...2500ppm	±5% of reading (-100...0hPa)
NO <sub>2</sub>	500...2500ppm	±5% of reading (-50...0hPa)
SO <sub>2</sub>	500...25000ppm	±5% of reading (-100...0hPa)
NO <sub>low</sub>	300...1500ppm	±5% of reading (-150...0hPa)
NO	1500...20000ppm	±5% of reading (-100...0hPa)
H <sub>2</sub> S	200...1500ppm	±5% of reading (-100...0hPa)
CxHy <sup>8, 9</sup>	The reading does not appear in the display	-
CO <sub>2</sub> -(IR)	The reading does not appear in the display.	-

---

<sup>6</sup> The additional measuring inaccuracy, that needs to be added to the measuring inaccuracy without dilution, is specified.

<sup>7</sup> Accuracy data are valid within the specified pressure range (pressure on probe tip).

<sup>8</sup> Detection limit: 50ppm

<sup>9</sup> Strict compliance with the lower explosion limit is mandatory.

### 3.2.8. Other instrument data

#### Flue gas analyser

Feature	Values
Ambient temperature	-5°C...45°C short-term (max. 5min.): up to 80°C by radiated heat (e.g. heat radiation from a hot exhaust channel)
Ambient pressure	600...1100mbar (abs.)
Ambient humidity	5...95%rF
Storage and transport temperature	-20 to 50°C
Degree of protection	IP40

#### Control unit

Feature	Values
Power supply	<ul style="list-style-type: none"> <li>• Li-ion rech. batt.</li> <li>• Meas. box</li> <li>• Mains adapter</li> </ul>
Battery charge time	7h (via mains adapter) 14h (via CAN interface)
Rech. batt. service life	approx. 5h (display switched on, Bluetooth® deactivated)
Memory	250,000 readings
Housing material	PC, TPE
Weight	440g
Display	Graphic colour display, 240 x 320 pixels
Dimensions	88 x 38 x 220mm

#### Analysis box

Feature	Values
Power supply	via rech. batt. Li-ion rech. batt. via internal mains unit: 100V AC/0.45A - 240V AC/ 0.2A (50-60Hz) via DC-input (option) 11V...40V DC/ 1 - 4A

### 3 Specifications

---

<b>Feature</b>	<b>Values</b>
Battery charge time	<6h
Battery operation time	2.5h (with gas cooler and IR module) / 4.5h (without gas cooler and IR module)
Dimensions	330 x 128 x 438mm
Housing	ABS URL 94V0
Weight	4800g (completely assembled)
Memory	250000 readings
Flue gas overpressure	max 50hPa
Underpressure	max. 300hPa
Pump volumetric flow rate	1 l/min (controlled), standard litre $\pm 0.1$ l/min
Hose length	max. 16.2m (corresponds to five probe hose extensions)
Diluting gas	Fresh air or nitrogen
Flue gas dust load	max. 20g/m <sup>3</sup>
Humidity load	max. 70°Ctd at measuring input
USB interface	USB 2.0
Trigger input	Voltage: 5...12V (falling or rising flank) Pulse width: >1 s Load: 5V/max. 5mA, 12V/max. 40mA
Bluetooth® option	Class1 module (reach <100m in open field)

## 4 Product description

### 4.1. Control Unit

#### 4.1.1. Overview



- 1 IrDA interface
- 2 Switch On / Off
- 3 Magnetic holder (on rear)

#### **⚠ WARNING**

Magnetic field

**May be harmful to those with pacemakers.**

- > Keep a minimum distance of 15 cm between pacemaker and instrument.

### ATTENTION





Magnetic field

#### **Damage to other devices!**


- > Keep a safe distance away from products which could be damaged by the effects of magnetism (e.g. monitors, computers or credit cards).

- 4 Display
- 5 Keyboard
- 6 Contact bar for meas. box (on rear)
- 7 Interfaces: USB 2.0, charger, Testo Data bus

### 4.1.2. Keyboard

Key	Functions
[  ]	Switch measuring instrument on / off
[OK] Example	Function key (orange, 3x), relevant function is shown on the display
[  ]	Scroll up, increase value
[  ]	Scroll down, reduce value
[esc]	Back, cancel function
[  ]	Open main menu
[i]	Open menu <b>Instrument diagnosis</b>

### 4.1.3. Display

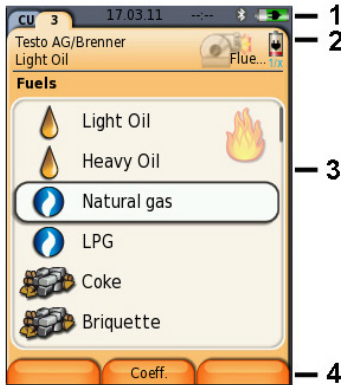

#### 1 Status bar (dark grey background):


- Display of date and time (valid for control unit and meas. box).
- Display of Bluetooth® status, power supply and remaining rech. batt. capacity (valid for control unit):

Icon	Feature
	<ul style="list-style-type: none"> <li>- Blue background / white symbol = Bluetooth® on, no Bluetooth® connection to the analyzer unit.</li> <li>- Grey background / white symbol = Bluetooth® off</li> <li>- Blue background / green symbol = Bluetooth® connection to meas. box up and running</li> </ul>
	<b>Battery operation</b> Indication of remaining capacity of the rech. batt. by colour and filling degree of the battery symbol (green = 20-100%, red = < 20%)
	<b>Mains operation</b> Indication of remaining capacity of rech. batt: see above

#### 2 Tabs and tab info field:

- Tabs: Display of measuring system components (CU = Control Unit, 2, 3, ... = meas. boxes, analog output box) connected to the Control Unit.

The tabs provide access to the individual components.

Warning symbol: 

- Red frame, red symbol / white background:  
Display of instrument errors in the instrument diagnosis menu, otherwise: Instrument designation.
  - Black frame, black symbol / yellow background:  
Information message (symbol is displayed alternately with the instrument designation).
  - Yellow frame, yellow symbol / red background:  
Warning (symbol is displayed alternately with the instrument designation).
- Information field on tab (only in the tabs of meas. boxes):  
Indication of selected folder/location, selected fuel, chosen application, status of power supply and remaining rech. batt. capacity (valid for meas. box, symbols like for display of Control Unit, see above), set dilution factor.
- 3 Selection field for functions (chosen function appears against a white background, unavailable functions are identified by grey characters) or display of measuring values.
  - 4 Function display for function keys.

### 4.1.4. Connections / interfaces



- 1 USB 2.0
- 2 Testo Data bus
- 3 Connecting socket for mains unit 0554 1096
- 4 Guide groove for locking with meas. box


### 4.1.5. Menu guidance for control unit

Main menu	Menu	Description
Measurement records	-	Display of saved measurement records
Device settings	Date/Time	Set date, time, time format:

<b>Main menu</b>	<b>Menu</b>	<b>Description</b>
	<b>Power Options</b>	Automatic instrument shut-down on / off Display backlight in battery operation on / off
	<b>Display brightness</b>	Set display brightness
	<b>Printer</b>	Select printer, enter print text
	<b>Bluetooth® (option)</b>	Bluetooth® on / off
	<b>Language</b>	Set instrument language
	<b>Country version</b>	Set country version
	<b>Password protection</b>	Change password
	<b>Data bus</b>	Display of bus address, enter bus rate
<b>Instrument diagnosis</b>	<b>Error diagnosis</b>	Display of present errors
	<b>Device information</b>	Display of device information
<b>Search for boxes</b>	-	Set up connection to meas. boxes

## 4.2. Meas. box

### 4.2.1. Overview

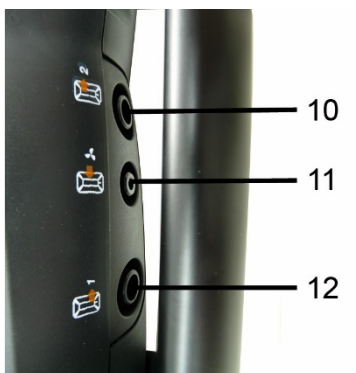

1 Condensate trap and condensate container,


- 2 Locking/unlocking button for Control Unit
- 3 Measuring gas particle filter
- 4 Filter fresh air inlet (option: fresh air valve / measurement range extension overall (5x))
- 5 Contact bar for connection to Control Unit
- 6 Guide pins for locking with Control Unit
- 7 Diluting gas filter
- 8 Status display
- 9 Full-view slider for marking/identification
- 10 Gas outlet 1
- 11 Fresh air inlet
- 12 Gas outlet 2

### 4.2.2. Status display

The status display shows the operating status of the meas. box:

Display	Status
green / permanent (meas. box switched on)	Operating status
red / flashing (meas. box switched on)	<ul style="list-style-type: none"> <li>• Rech. batt. operation / residual rech. batt. capacity &lt; 20%</li> <li>• other device error</li> </ul>
green / off / yellow, each flashing alternately for 1 second	Rechargeable battery is charging or trickle charging, measurement program is waiting for program start, instrument is in standby mode
green, red / alternately flashing	Update mode active
green, yellow alternately flashing (green is on longer)	Instrument is in the switch-on phase
yellow, green alternately flashing (yellow is on longer)	Instrument is in the switch-off phase

### 4.2.3. Connections / interfaces

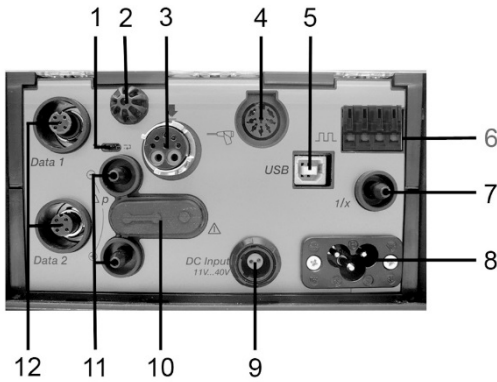

- 1 Data bus termination slide switch
- 2 Sensor for combustion air temperature
- 3 Flue gas probe
- 4 Sensor input
- 5 USB 2.0
- 6 Trigger input
- 7 Dilution gas inlet for measurement range extension
- 8 Mains connection 100...240V AC, 50-60Hz
- 9 DC-voltage input 11...40V DC (option)
- 10 Covering cap gas channel access (only for servicing purposes)




Plugged in covering cap: Position (●—● ●) must not be changed!

- 11 Pressure ports p+ and p-
- 12 Testo Data bus

### 4.2.4. Functions / instrument options

Some functions are available as optional extras. The functions your meas. box is equipped with (condition as delivered) can be read on the identification plate on the bottom side of the meas. box.

Imprint	Description
CO, NO, NO <sub>2</sub> , SO <sub>2</sub> , NO <sub>low</sub> , CO <sub>low</sub> , CxHy, H <sub>2</sub> S, O <sub>2</sub> , CO <sub>2</sub> -(IR)	The sensor of the specified type is plugged in

<b>Imprint</b>	<b>Description</b>
SG	Special main gas pump for long-term measurement
1/x	Measurement range extension (individual dilution with selectable dilution factors)
DC	DC-voltage input (11...40V DC)
$\Delta p=0$	Automatic pressure zeroing for flow measurement
GP	Gas preparation, by means of reduced and constant measuring gas dew point temperature for higher measuring accuracy
	Fresh air valve for overall dilution (x5) to measure high flue gas values.


#### 4.2.5. Menu guidance meas. box

<b>Main menu</b>	<b>Menu</b>	<b>Description</b>
<b>Applications</b>	-	Select an application in accordance with the measuring task to be performed
<b>Folders</b>	-	Create and manage folders and locations
<b>Fuels</b>	-	Select and configure fuels
<b>Measurement records</b>	-	Display and manage measurement records

## 4 Product description

<b>Main menu</b>	<b>Menu</b>	<b>Description</b>
<b>Device settings</b>	<b>Dilution</b>	Set the dilution factor
	<b>Measurement view</b>	Configure the display, set measurement parameters and units for selected application and measurement type
	<b>Units</b>	Set units for display variables
	<b>Date / time</b>	Set date, time, time format:
	<b>Power Options</b>	Set automatic instrument shut-down and switch off display backlight in rech. batt. operation
	<b>Display brightness</b>	Set display brightness
	<b>Printer</b>	Select printer, enter print text
	<b>Bluetooth®</b>	Bluetooth® on / off
	<b>Language</b>	Set instrument language
	<b>Country version</b>	Set country version (fuels, display variables, calculation formulas)
	<b>Password protection</b>	Change password
	<b>Analog input</b>	Configure analog input
	<b>Databus</b>	Display of bus address, enter bus rate
<b>Sensor settings</b>	-	Make sensor settings, perform calibration / adjustment
<b>Programs</b>	-	Configure and activate measuring programs
<b>Instrument diagnosis</b>	<b>Error diagnosis</b>	Display of present errors
	<b>Gas path check</b>	Perform tightness test
	<b>Sensor diagnosis</b>	Perform sensor diagnosis
	<b>Device information</b>	Display of device information

#### 4.2.6. Modular flue gas probe

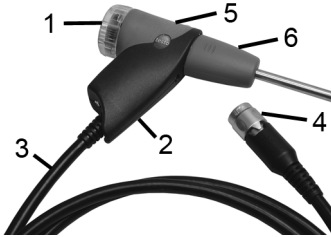

- 1 Removable filter chamber with window and particle filter
- 2 Probe handle
- 3 Connecting cable
- 4 Connector plug for measuring instrument
- 5 Probe module lock release
- 6 Probe module

## 5 First steps

### 5.1. Commissioning

#### **Control Unit**

The Control Unit has a permanently installed rechargeable battery.

- > Remove the protective film from the display.
- > Charge the rech. batt. fully before using the Control Unit.

#### **Meas. box**

The meas. box is supplied with a rech. batt. already fitted.

- > Charge the rech. batt. fully before using the meas. box.

### 5.2. Getting to know the product

#### 5.2.1. Mains unit, batteries/rechargeable batteries

---



In case of longer interruption of the power supply to the Control Unit (e.g. rech. batt. empty) the settings for date / time will be lost.

---

##### 5.2.1.1. Recharging the rech. batt. of the Control Unit

The rech. batt. can only be charged at an ambient temperature of  $\pm 0...+35^{\circ}\text{C}$ . If the rech. batt. had been completely discharged, the charging time at room temperature will take about 7h (charging with mains adapter) or approx. 14h (charging via Testo Data bus).

---



In the case of Testo data bus cables >90 m, the rechargeable battery for the control unit can no longer be charged via the Testo data bus cables when the control unit is switched off. In this case the external mains unit 0554 1096 is required in order to charge the battery.

The CU can be used without an external mains unit during operation, even with Testo data bus cables >90 m.

---



testo data bus cables must not be used during electrical storms.

---

**Charging via mains unit (Art.-No. 0554 1096)**

- ✓ The Control Unit is switched off.
- 1. Connect the plug of the mains unit to the mains unit socket on the Control Unit.
- 2. Connect the mains plug of the mains unit to a mains socket.
  - The charging process starts. The charge condition will be shown on the display.
  - Once the rech. batt. has been charged the instrument will automatically change to trickle charge.

**Charging via meas. box**

- ✓ Control Unit is locked to meas. box or is connected via the Testo Data bus cable.
- ✓ The meas. box is supplied via the mains unit.

During operation with low charge power or in switched off state.

**5.2.1.2. Charging the rech. batt. of the meas. box**

The rech. batt. pack can only be charged at an ambient temperature of  $\pm 0 \dots +35^{\circ}\text{C}$ . If the rech. batt. has been discharged completely, the charging time at room temperature is approx. 6h.

- ✓ The meas. box is switched off.
- > Connect mains cable to meas. box and mains socket.

**5.2.1.3. Battery care**

- > Do not fully exhaust rechargeable batteries.
- > Store rech. batts. only in charged condition and at low temperatures, but not below  $0^{\circ}\text{C}$ .
- > For longer breaks you should discharge and recharge the batteries every 3- months. Trickle charging should not exceed 2 days.

**5.2.1.4. Mains operation**

In case of danger the instrument must be disconnected from the electric power supply by simply pulling out the mains cable.

- > Always position the instrument so that the power supply plug can be easily reached.

**Control Unit**

1. Connect the plug of the mains unit to the mains unit socket on the Control Unit.
2. Connect the mains plug of the mains unit to a mains socket.

- The Control Unit is powered by the mains unit.
- If the Control Unit is switched off the rech. batt. charging process will start automatically. Switching the Control Unit on has the effect of stopping battery charging and the Control Unit being powered via the mains unit.

### **Meas. box via internal mains unit**

- > Connect the mains cable to meas. box and mains socket.
- The meas. box is powered via the internal mains unit.
- If the meas. box is switched off the rech. batt. charging process will start automatically. Battery charging stops when the flue gas analyser is switched on by the Control Unit.

### **Meas. box via DC-voltage input DC**

- ✓ Cable with battery terminals and adapter for connection to meas. box required (0554 1337, accessory).
- If the meas. box is switched off the rech. batt. charging process will start automatically. Battery charging stops when the flue gas analyser is switched on by the Control Unit.

## **5.2.2. Connecting probes / sensors**

---



Sensor detection takes place during the activation process: Sensors that are required must always be connected before the flue gas analyser is switched on, or the flue gas analyser must be switched off and then on again after a sensor change, so that the correct sensor data can be read.


---

- > Connect the required probes / sensors to the corresponding ports.


## **5.2.3. Occupying the trigger input**

The trigger input can be used as a criterion to either start or stop (ascending or descending flank) measuring programs.

- > Occupying the trigger input, with external voltage supply (5...12 V):

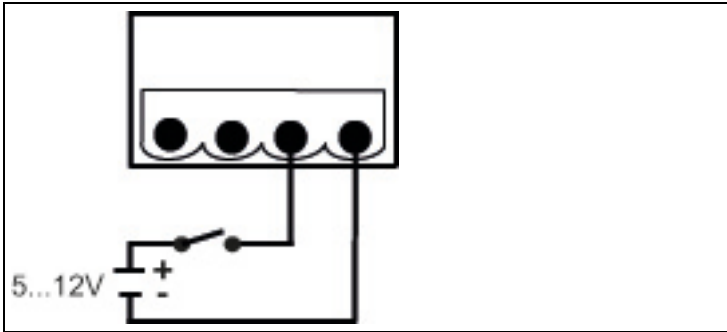

- > Occupying the trigger input, with supply via instrument voltage (12 V):

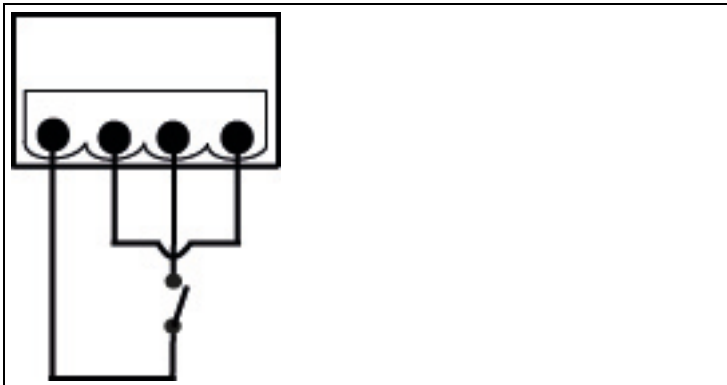

**i** In case of supply via instrument voltage the flue gas analyser can only be started via the trigger input from switched off state when the mains plug is plugged in.

## 5.2.4. Connecting system components

### 5.2.4.1. Connection using contact strip



The Control Unit can be plugged onto the meas. box.

1. Place the guide groove in the bottom side of the Control Unit over the guide pins of the meas. box.
2. Press the Control Unit against the meas. box until the locking/unlocking buttons noticeably clicks into place **two times**.

---

**i** To protect the display (e.g. during transport) the Control Unit can also be inserted with the back facing up, however, in this case there is no connection to the meas. box.

---

### 5.2.4.2. Connection using a Data bus cable (accessory part to a bus system)

---

**i** testo data bus cables must not be used during electrical storms.

---

---

**i** Before connecting to a bus system, all analyzer units must first be equipped with the identical country version and firmware version.

---



or



**i** If testo easyEmission software is connected via a control unit to measuring boxes, the number of measuring boxes must not be changed. To add new measuring boxes, end the testo easyEmission software, connect the new measuring box and restart the testo easyEmission software.

or



or




The individual components (e.g. Control Unit with meas. box or meas. box with meas. box) can be connected to a bus system using the Testo Data bus cable.

**i** Prior to commissioning a bus system, the bus address, bus rate, application and measuring location must be configured separately in each analyzer box and measurement programs which are running or active must be deactivated in each individual analyzer box.

For this, before the components are connected to a bus system, each component must be configured separately either with the control unit or the notebook/PC.

Calling up the function:

 → **Device settings** → **[OK]** → **Data bus** → **[OK]**.

### Bus address

The bus address of each component connected to the Testo data bus must be unambiguous. The bus address of the connected component can be changed, if necessary.

1. **Bus Address** → [Edit].
2. Setting a new bus address: [▲], [▼], [◀], [▶].
3. Confirm the entry: [OK].

### Bus rate

The relevant data rate must be selected depending on the number of connected components in a system.

- Control unit with one measuring box: **500 kbit/s**
  - All other systems: **50 kbit/s**
- > Select **bus rate 500 kbit/s** or **50 kbit/s**: [▲], [▼], → [Edit] → [📄] or [ESC].

---

**i** If several meas. boxes are connected with the Control Unit, only the measurement data from one meas. box can be displayed at a time, or only one meas. box can be activated respectively. This is accomplished by selecting the meas. box, see **Search for meas. boxes**, page 43.

**i** If several meas. boxes are connected to a notebook/PC, the meas. boxers can be activated and opened parallel to each other, e.g. to display measuring channels of different meas. boxes parallel to one another.

---

**i** If a notebook/PC or data bus controller (0554 0588) has several connected and enabled measuring boxes, the minimum measuring rate changes, depending on the number of measuring boxes, as follows:

Measuring boxes	Minimum measuring rate
1 to 2	1 s
3 to 4	2 s
5 to 8	3 s
9 to 16	5 s

---

> Connect the Data bus cable to the Data bus interfaces. Please observe the following points when setting up a connection via Data bus cable:

- Use only Testo databis cables

- Do not route Data bus cables in the vicinity of electric power cables.
- Ensure sufficient power supply by supplying each meas. box with mains voltage.
- The cables should ideally be plugged in before the system is switched on. Connecting during operation (hot plugging) is possible, however, depending on the combination the system may need to be switched off and on again.
- The connection cannot be separated under load.
- Data bus subscribers: max. 16 meas. boxes in one Data bus system.
- Cable length: max. 100 m between Control Unit and meas. box, max. 800 m between all meas. boxes in the Data bus system.
- The bus system must have a defined electrical termination, see below.

### Electrical termination of the bus system


The Data bus system is linear in structure. The Control Unit or the Testo Data bus controller with USB connection represents the beginning of the line.

The end is represented by the last components connected in the system (meas. box or analog output box). This component must have a defined electrical termination.

An analog output box is the furthest subscriber.

- > Plug the Data bus termination plug into the Data bus socket on the analog output box.

A meas. box is the furthest subscriber.

- > Set the Data bus terminating slide switch on the meas. box (see Connections / interfaces page 28, point 1) to switch position right (  ).

### 5.2.4.3. Connection via Bluetooth® (option)



or



or



Via Bluetooth® the Control Unit can be connected to a meas. box or a PC/Notebook, as long as both components are equipped with this function, see **Bluetooth®**, page 56.

---

**i** The Bluetooth® connection between measurement box and PC/computer is no longer supported for Windows® XP.

---

### 5.2.5. Switching on


#### Before switching on

- > Connect all system components.
- > Connect all required probes / sensors.
- > Connect all system components to the electric power supply.

When switching on the Control Unit

- should be plugged on the contact strip of the meas. box
- or
- connected with a Data bus cable
- or
- plugged to the mains cable of the meas. box, so that starting via Bluetooth® is enabled.

#### Switching on

- > press .

- The Welcome Screen is displayed (approx. 5s)
- The Control Unit display screen appears.
- The Control Unit searches for connected meas. boxes and shows these as independent tabs in the display.

---

**i** Control Unit and meas. box are not connected:  
If the Control Unit has already been switched on, you must press **[⏻]** once again for a short moment to set up a connection to the meas. box.

---


## 5.2.6. Calling up a function

1. Select function: **[▲]**, **[▼]**.
  - The chosen function appears in a frame.
2. Confirm selection: **[OK]**.
  - The chosen function is opened.

## 5.2.7. Entering values

Some functions require values (numbers, units, characters) to be entered. Depending on the function that is chosen, the values are entered via either a list field or an input editor.

### List field

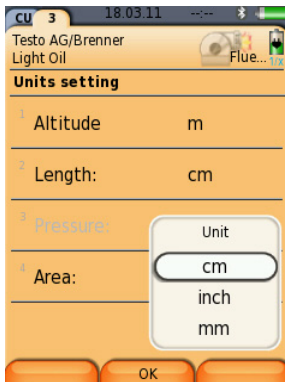

1. Select the value to be changed (numerical value, unit): **[▲]**, **[▼]**, **[◀]**, **[▶]** (depending on the selected function).
2. Press **[Change]**.
3. Set value: **[▲]**, **[▼]**, **[◀]**, **[▶]** (depending on the selected function).
4. Confirm the entry: **[OK]**.
5. Repeat steps 1 and 4 as required.

6. Save the entry: **[Finished]**.

**Input editor**



1. Select the value to be changed (character): **[▲], [▼], [◀], [▶]**.
2. Accept value: **[OK]**.

Options:

- > Toggle between characters and special characters:

Select |← **ABC→&\$/** →|: **[▲], [▼]** → **[ABC→&\$/]**.

- > Position the cursor in the text:

Select |← **ABC→&\$/** →|: **[▲], [▼]** → **[|←]** or **[|→]**.

- > Delete character after the cursor:

Select |← **ABC→&\$/** →|: **[←]** or **[→]** → **[▼]** → **[Del]**.

- > Delete character in front of cursor:

Select |← **ABC→&\$/** →|: **[←]** or **[→]** → **[▼]** → **[←]**.

3. Repeat steps 1 and 2 as required.
4. Save the entry: Select **← Finished →**: **[▲], [▼]** → **[Finished]**.

**5.2.8. Printing / saving data**

Printing and saving is accomplished via the menu **Options**, which is accessed via the left function key and is available in many different menus.

Assignment of the right function key with the function **Save** or **Print**, see Assigning the right hand function key page 50.

---

**i** When an IRDA printer 0554 0549 is used, the control unit must not be placed on the analyzer box during the printout.

---

**i** Only readings, which have a display field in the measurement view assigned, will be saved / printed out.

---

**i** The measurement data can be printed out parallel to the saving process, while a measurement program is running.

---

**i** Measure values of diluted sensors (with enabled measurement range extension) underlined on the printout.

---

### 5.2.9. Search for meas. boxes

(only available via **Control Unit** tab)

>  → **Search for boxes** → **[OK]**.

- Meas. boxes connected via Testo Data bus: are displayed (tabs)
  - Meas. boxes connected via Bluetooth®:
    - Meas. box found:  
Meas. box and Control Unit are connected automatically
    - several meas. boxes found:  
The available meas. boxes are displayed for selection
- 

**i** An existing Bluetooth® connection is disconnected by selecting a new meas. box from the selection field.

---

### 5.2.10. Confirming an error message

If an error occurs, an error message is shown in the display.

> Confirming an error message: **[OK]**.

Errors which have occurred and have not yet been rectified are indicated by a warning symbol in the status bar.

Not yet rectified error messages can be displayed in the menu **Error diagnosis**, see Sensor diagnosis, page 48.

### 5.2.11. Switching off


---

**i** Unsaved readings will be lost when the flue gas analyser is switched off.

---

#### Rinse phase

When switched off, the meas. box checks whether flue gases are still in the sensors. The sensors are rinsed with fresh air, if this should be necessary. The duration of the rinse phase depends on the gas concentration in the sensors.

- > press .
- The rinse phase starts.
- The flue gas analyser switches off. It is normal for the fan of the meas. box to run on for a while.

### 5.3. Folders / Locations

(only available via **Meas. Box** tab)

All readings can be saved under the currently active location. Readings not yet saved are lost when the measuring instrument is switched off.

Folders and locations can be created, edited, copied and activated. Folders and locations (incl. protocols) can be deleted.

Calling up the function:

- >  → **Folders** → **[OK]**.

Adapting the display:

- > Toggle between overview (display of number of locations per folder) and detailed view (display of all locations per folder): **[Overview]** or **[Details]**.

Activating a location:

- > Select the location → **[OK]**.
- The location is activated and the menu **Measurement Type** is opened.

Creating a new location:

A location is always created in a folder.

1. Select the folder in which the location is to be created.
2. **[Options]** → **New location** → **[OK]**.
3. Enter values or make settings.

The following inputs/settings are possible:

Parameter	Description
<b>Location</b>	Enter name
<b>Application</b>	Select application
<b>Fuel</b>	Select fuel
<b>Profile</b>	Enter diameter, length, width, height and area. For correct measurement of the volume flow you must set the profile and area. A volumetric flow rate is calculated from the geometries entered here together with the measured velocity.

Parameter	Description
<b>Pitot Tube Factor</b>	<p>The parameter "Pitot tube factor" influences the measurement of flow speed, volume flow rate and mass flow. The Pitot factor depends on the type of Pitot tube used:</p> <p>Straight Pitot tubes: Factor = 0.67 Prandtl Pitot tubes (bent): Factor = 1</p>
<b>Humidity</b>	<p>The parameter "Humidity" (combustion air humidity) influences the calculation of qA (flue gas loss) and flue gas dew point. The factory setting is 80.0% humidity. To achieve a higher accuracy, the values can be adjusted to the actual ambient conditions.</p>
<b>Pressure absolute</b>	<p>The absolute pressure influences the calculation of flow speed, volume flow, mass flow and flue gas dew point. The factory setting is 980mbar. To achieve a higher accuracy, the values can be adjusted to the actual ambient conditions.</p> <hr/> <p><b>i</b> If a CO<sub>2</sub>-(IR) module is installed, the absolute pressure value measured there will automatically be used.</p>
<b>Barometric pressure</b>	<p><b>i</b> The input of the barometric pressure and the height above sea level is only required when no absolute pressure is available (no CO<sub>2</sub> IR module present).</p> <hr/> <p>The barometric pressure influences the calculation of flow speed, volume flow, mass flow and flue gas dew point. To achieve a higher accuracy, the values can be adjusted to the actual ambient conditions.</p> <p>This is 1013mbar as an annual average, regardless of the altitude. Depending on the current weather, this pressure can fluctuate by ±20mbar around the annual average.</p>
<b>Altitude</b>	<p>The height above sea level influences the calculation of flow speed, volume flow, mass flow and flue gas dew point. To achieve a higher accuracy, the value can be adjusted to the actual ambient conditions.</p>

Parameter	Description
Dewpoint	The parameter "Dewpoint" (combustion air dewpoint) influences the calculation of qA (flue gas loss) and flue gas dew point. The factory setting for the dewpoint is 1.5°C. To achieve a higher accuracy, the values can be adjusted to the actual ambient conditions.

4. Finalise the entry: **[Finished]**.

**Other location options:**

- > **[Options]** → **Edit location**: Make changes to an existing location.
- > **[Options]** → **Copy location**: Make a copy of an existing location in the same folder.
- > **[Options]** → **Delete location**: Delete an existing location.

Create a new folder:

1. **[Options]** → **New Folder** → **[OK]**.
2. Enter values or make settings.
3. Finalise the entry: **[Finished]**.

**Other folder options:**

- **Edit Folder**: Make changes to an existing folder.
- **Copy Folder**: Make a copy of an existing folder.
- **Delete Folder**: Delete an existing folder, including the locations created therein.
- **Delete All Folders**: Delete all existing folders, including the locations created therein.

## 5.4. Measurement records

**Meas. box**

Measurement data are always saved in a measurement record in the meas. box with which the measurement data were measured.

An overview with all created folders and locations is displayed. The measurement records saved for the corresponding locations are displayed. Measurement records can be displayed, printed, deleted and copied to the Control Unit.


**Control Unit**

Locations cannot be saved in the Control Unit. Measurement records saved in the meas. box can be copied to the Control Unit,

e.g. to be able to transport these for evaluation by PC software, while the meas. box remains at the location.

For easy assignment the measurement records are saved under the serial number of the meas. box. The data (folders, locations, readings) contained in these records are displayed like in the meas. box.

Calling up the function:

- >  → **Measurement Records** → **[OK]**.
- > only with Control Unit tab: Choose the serial number of the meas. box → **[OK]**.

Adapting the display:

- > Toggle between overview (display of number of locations per folder) and detailed view (display of all locations per folder): **[Overview]** or **[Details]**.

### Display record:

1. Choose the desired record from the detailed view.
2. **[Data]**.

### Options

- > **[Options]** → **[Delete All Records]**: The readings of all locations will be deleted.
- > **[Options]** → **[Copy All Records]**: The readings of all locations will be copied.

### Meas. box options

- > **[Options]** → **Print Data**: Transmit data of the chosen record to a record printer.
- > **[Options]** → **Copy Record**: Copy record into the record log of the Control Unit.
- > **[Options]** → **Delete Record**: Delete the chosen record.
- > **[Options]** → **Show Graphic**: Display saved record data as graphic.
- > **[Options]** → **Number of lines**: Change the number of measuring values per display page.
- > **[Options]** → **Delete All Records**: Delete all saved records for a location.
- > **[Options]** → **Copy All Records**: Copy all records of a location into the record log of the Control Unit.

### Control Unit options

- > **[Options]** → **Delete All Records**: Delete all saved records for a location.

## 5.5. Instrument diagnosis

Important operating values and instrument data are displayed. A gas path check can be carried out. The status of the sensors and any device errors not yet rectified are displayed.

Calling up the function:

- >  → **Instrument diagnosis** → [OK].
- or
- > [i].

### 5.5.1. Error diagnosis

- > **Error diagnosis** → [OK].
- Unrectified errors, warnings and notes are displayed.
  - > View next / previous error: [**▲**], [**▼**].

### 5.5.2. Gas path check

(only available via **Meas. Box** tab)

Check the flue gas analyser regularly for leaks, to ensure accurate measurements.

The leak test requires a plastic cap 0193 0039, comes with the flue gas probe).

1. **Gas path check** → [OK]
2. Place the plastic cap on the tip of the flue gas probe so that the openings are completely covered.
  - The pump flow is displayed.
  - Volumetric flow rate less than or equal to 0.04l/min: The gas paths are leak tight (traffic light in display lights green).
  - Volumetric flow rate higher than 0.04l/min: The gas paths are leaking (traffic light in display lights red). Probe and meas. box must be checked for leaks.

### 5.5.3. Sensor diagnosis

(only available via **Meas. Box** tab)

1. **Sensor diagnosis** → [OK].
2. Select sensor. [**▲**], [**▼**].
  - The status of the sensor is indicated by a lamp.



A sensor is able to recover. It is therefore possible that the sensor status indication changes from yellow to green or from red to yellow.

---

#### 5.5.4. Instrument information

- > **Device information** → [OK].
  - Information is displayed.
- 



The fill level of the condensate trap is only displayed if the condensate trap is plugged onto the analyzer unit.

---

## 6 Using the product

### 6.1. Performing settings

#### 6.1.1. Assigning the right hand function key

The right function key can have a function from the **Options** menu assigned to it. The menu **Options** is accessed via the left function key and is available in many different menus. This assignment is only valid for the currently opened menu / the opened function.

- ✓ A menu / function is opened in which the **Options** menu is displayed on the left function key.

1. Press **[Options]**.
2. Select option: **[▲]**, **[▼]**.

Depending on the menu / function from which the **Options** menu was opened, various functions are available.

3. Assign the selected function to the right function key: Press the **[Config. Key]**.

#### 6.1.2. Instrument settings

##### 6.1.2.1. Dilution

(only available via tab **Meas. Box** and with the measurement range extension option)

##### **Option dilution (for single slot with selectable dilution factors**

With active dilution the measuring gas for the sensor in slot 6 is diluted with ambient air (other possibility: nitrogen gas) in a controlled manner. For this purpose, the diluting gas is drawn through a separate gas inlet by a pump and a valve operating on the principle of pulse width modulation. A filter is installed to protect the gas path against dust.

If the measurement range extension is active this is indicated by a clearly noticeable clicking of the valve. In addition the symbol 1/x appears at the right hand top of the display (in the header) and the selected dilution factor appears at the corresponding parameter (the complete line of the diluted parameter appears against a blue background).

The following dilution factors can be manually set:

Factor	Ratio of diluting gas: Measuring gas
x 1	no dilution
x 2	1 : 1
x 5	4 : 1
x 10	9 : 1
x 20	19 : 1
x 40	39 : 1
Auto dilution	4 : 1

If the dilution stage **auto-dilution** is selected, dilution (5x) is activated automatically when the set switch-off threshold of the sensor in slot 6 is reached.



- If the surrounding air contains interfering gases, push the hose onto the dilution inlet and place in a clean atmosphere.
- If gas from a gas cylinder is used, observe a max. pressure of 30hPa
- Diluting also changes the resolution of the reading display, e.g.:  
Undiluted resolution 1ppm, with factor 10 resolution 10ppm.

Calling up the function:

> → **Device settings** → **[OK]** → **Dilution** → **[OK]**

1. **Single slot** → **[Change]**

2. Set the dilution factor: , .

3. Confirm the entry: **[OK]**.

Option:



> Without dilution: Press **[Without]**.

### Measurement range extension with fixed dilution factor (x5) for all sensors (fresh air valve option)

The selection of **to dilute all** (x5) results in the dilution of all sensors (x5). The measuring channels O<sub>2</sub>, CO<sub>2</sub>-(IR), CO<sub>2</sub>, qA, Lambda, Eta and all measuring channels for flow measurements are faded out in case of dilution **to dilute all**. 1x deactivates the dilution (extension of measuring range).

It is possible to calibrate / adjust with test gas when dilution is switched on to eliminate any measuring errors caused by dilution (see Calibration / adjustment page 61).

Calling up the function:

- >  → **Device settings** → **[OK]** → **Dilution** → **[OK]**
1. Select **to dilute all (x5)**:  → **[Change]**.
  2. Select setting: **[On]** / **[Off]**.
  3. Confirm the entry: **[OK]**.

### 6.1.2.2. Measurement view

(only available via **Meas. Box** tab)

The parameters / units and the display representation (number of readings displayed per display page) can be set.

The settings are only valid for the currently chosen combination of application and measurement type, which is indicated by the symbol (application) and the text (measurement type) in the info field.



Only those parameters and units that are activated in the reading display appear in the reading display, in the saved measurement records and on the record printouts. Readings not listed in the reading display are not recorded or stored either. Before carrying out measurements, set up the reading display so that the required measurement parameters and units are enabled.

Total overview of selectable parameters and units (available selection depends on the chosen application / measurement type):

Display	Measurement parameter
<b>FT</b>	Flue gas temperature
<b>AT</b>	Combustion air temperature
<b>HCT</b>	Heat carrier temperature
<b>Δp</b>	Differential pressure
<b>Δp1</b>	Differential pressure 1 (flue gas + m/s)
<b>Δp2</b>	Differential pressure 2 (flue gas + ΔP)
<b>Draught</b>	Flue draught
<b>Pabs</b>	Absolute pressure
<b>Pump</b>	Pumping capacity
<b>O2</b>	Oxygen
<b>CO2</b>	Carbon dioxide
<b>CO2max</b>	maximal carbon dioxide content
<b>Effn</b>	Efficiency

<b>Display</b>	<b>Measurement parameter</b>
<b>Effg</b>	Efficiency under due consideration of the heat value range
<b>CO</b>	Carbon monoxide
<b>uCO</b>	Carbon monoxide undiluted
<b>AmbCO</b>	Ambient carbon monoxide
<b>NO</b>	Nitrogen monoxide
<b>NO2</b>	Nitrogen dioxide
<b>NOx</b>	Nitrogen oxide
<b>SO2</b>	Sulphur dioxide
<b>H2S</b>	Hydrogen sulphide
<b>HC</b>	Hydrocarbon
<b>H2</b>	Hydrogen (this is only an indicator value and is used to compensate the cross-sensitivity)
<b><math>\lambda</math></b>	Air ratio
<b>Smoke numberØ</b>	Mean smoke number
<b>Oil deposits</b>	Oil deposits yes/no
<b>Ratio</b>	Poison index
<b>Vel</b>	Flow velocity
<b>Volume flow</b>	Volume flow
<b>Dew Pt</b>	Flue gas dew point temperature
<b>MCO</b>	Mass flow CO
<b>MNOx</b>	Mass flow NOx
<b>MSO2</b>	Mass flow SO <sub>2</sub>
<b>MH2S</b>	Mass flow H <sub>2</sub> S
<b>CO2IR</b>	Carbon dioxide IR active
<b>MCO2IR</b>	Mass flow CO <sub>2</sub> -IR
<b>AmCO2</b>	Ambient carbon dioxide
<b>%rH ambient</b>	Humidity measuring value external sensor
<b>UI ext</b>	external voltage
<b>Itemp</b>	Instrument temperature

Calling up the function:

>  → **Device settings** → **[OK]** → **Measurement view** → **[OK]**

Change parameter / unit in a line:

1. Select the line: [▲], [▼] → [Change]
2. Select the parameter: [▲], [▼] → [OK]
3. Select the unit: [▲], [▼] → [OK]
4. Save changes: [OK]

### Options:

- > [Options] → **Number of lines**: Change the number of measuring values per display page.
- > [Options] → **Blank line**: Insert the empty line before the selected line.
- > [Options] → **Delete line**: Delete the selected line.
- > [Options] → **Factory setting**: Reset the readings display to factory setting.

### 6.1.2.3. Units

(only available via **Meas. Box** tab)

The units used for parameters in configuration menus can be set.

Calling up the function:

- > [Menu] → **Device settings** → [OK] → **Units** → [OK]

#### Adjustable units

Parameter	Unit
<b>Altitude</b>	m, ft
<b>Length</b>	cm, inch, mm
<b>Pressure</b>	mbar, psi, inHG, inW, hPa
<b>Area</b>	mm <sup>2</sup> , in <sup>2</sup>
<b>Volume</b>	m <sup>3</sup> , l
<b>Volume flow</b>	m <sup>3</sup> /h, l/min
<b>Time</b>	sec, min

#### Setting the unit

1. Select the line: [▲], [▼] → [Change].
2. Select the unit: [▲], [▼] → [OK].
3. Confirm the entry: [Finished]

#### 6.1.2.4. Date / time

This function is available in both the meas. box and the Control Unit. Changes are accepted for the Control unit and for the meas. box.

Date, time mode and time can be set.

Calling up the function:

>  → **Instrument Settings** → [OK] → **Date/Time** → [OK]

##### Set date/time

1. Select parameter: [**◀**], [**▲**], [**▼**] → [Edit].
2. Set parameter: [**▲**], [**▼**] and partly [**◀**], [**▶**] → [OK].
3. Save changes: [Save].

#### 6.1.2.5. Power options

This function is available in both the meas. box and the Control Unit. Changes are accepted by the Control Unit and the meas. box.

Automatic instrument shut-down (Auto-Off) and switching off of the display light in battery operation can be set.

Calling up the function:

>  → **Device settings** → [OK] → **Power Options** → [OK]

##### Making settings:

1. Select function or parameter: [**▲**], [**▼**] → [Change]
2. Set parameter: [**▲**], [**▼**] and partly [**◀**], [**▶**] → [OK].
3. Save changes: [Finished]

#### 6.1.2.6. Display brightness

This function is available in both the meas. box and the Control Unit. Changes are accepted for the Control unit and for the meas. box.

The intensity of the display illumination can be set.

Calling up the function:

>  → **Instrument Settings** → [OK] → **Display Brightness** → [OK]

Performing settings

> Set parameter: [**◀**], [**▶**] → [OK].

#### 6.1.2.7. Printer

This function is available in both the analyzer unit and the control unit. Changes are accepted for the control unit and for the analyzer unit.

The headers (lines 1-3) and the footer for the printout can be set. To be able to transfer data to a record printer via infrared or Bluetooth interface, the printer used must be enabled.

The following printers can be used with the testo 350:

- infrared high-speed printer (order no. 0554 0549)
- Bluetooth®/IRDA printer (order no. 0554 0620)

Calling up the function:

>  → **Instrument Settings** → [OK] → **Printer** → [OK]

### Activating the printer:

---



The printer 0554 0620 can only be selected after the Bluetooth®-interface has been activated, see **Bluetooth®**, page 56.

---

1. **Select Printer** → [OK].
2. Select the printer: [**▲**], [**▼**] → [OK].
- The printer is activated and the menu **Printer** is opened.

### Setting the print text:

1. **Print text** → [OK].
2. Select function: [**▲**], [**▼**] → [Edit].
3. Enter values → [Next].
4. Save the entry: [Finished].

### 6.1.2.8. Bluetooth®

This menu is only available if the instrument is equipped with Bluetooth® option. The Bluetooth module can be switched on / off. This function is available in both the meas. box and the Control Unit. Settings only apply for the device activated at the time.



To set up a connection between Control Unit and meas. box, see **Connection via Bluetooth®** (option), page 39.

To set up a connection between Control Unit and Notebook/PC: Follow the operating instructions for the software and Notebook/PC used.

Calling up the function:

>  → **Device settings** → [OK] → **Bluetooth®** → [OK].

### Switching Bluetooth® on / off

1. [Change].
2. Select setting: [, ] → [OK].
3. Confirm the entry: [Finished].

### 6.1.2.9. Language

This function is available in both the meas. box and the Control Unit. Changes are accepted for the Control Unit and for the meas. box.

The menu language can be set. The number of available languages depends on the activated country version, see Country version, page 57.

Calling up the function:

>  → **Device settings** → [OK] → **Language** → [OK]

#### Activate the language:

> Select the language → [OK].

### 6.1.2.10. Country version

This function is available in both the meas. box and the Control Unit. Changes are accepted for the Control Unit and for the meas. box.

The country version can be set. The selection of the country version influences the menu languages that can be activated.

Please make sure that the correct country version has been set.

By changing the country version the bases of calculation and thus the displayed measurement parameters, fuels, fuel parameters and calculation formulas may change.

Information concerning assignment table, basis of calculation and country version see [www.testo.com/download-center](http://www.testo.com/download-center)



If several components with different country versions are connected, the components will automatically change to the country version of the Control Unit when the Control Unit is connected.

---

Calling up the function:

>  → **Device settings** → [OK] → **Country Version** → [OK]



This action can be password protected. A password is specified in the menu **Password protection**, see Password protection, page 58.

---

Possibly:

> Enter the password: [Enter] → Enter password → [Next] → [OK].

#### Setting the country version:

1. Select the country version: [▲], [▼] → [OK].

2. Confirm confirmation request: **Yes** → **[OK]**
  - The system is restarted.



---

**i** If the control unit is connected via Bluetooth to the measuring box, when the measuring box is restarted, the control unit should be used to search again for the measuring box (see **Search for meas. boxes**, page 43.)

---

### 6.1.2.11. Password protection

This function is available in both the meas. box and the Control Unit. Changes are accepted for the Control unit and for the meas. box.

The password protection is only valid for functions identified by the following symbol:  or .

Password protection can be activated / deactivated, the password can be changed.

To deactivate the password protection change the password to **0000** (factory setting).

Calling up the function:

- >  → **Instrument Settings** → **[OK]** → **Password Protection** → **[OK]**

Possibly:

- > Enter the currently valid password:  
**[Enter]** → Enter password → **[Next]** → **[OK]**.

**Changing the password:**

1. **[Edit]**.
2. Enter the new password → **[Next]**.
3. **[Edit]**.
4. Enter the new password again to confirm → **[Next]**.
5. Save changes: **[Finished]**.

### 6.1.2.12. Analog input

(Only available via **Meas. Box** tab)

Power cable 0554 0007 (accessory) is required.

An analog signal is read in by an external instrument. The signal is scaled and assigned to a physical parameter. The calculated value is displayed.

---

**i** Before the flue gas analyser is started, insert power cable 0554 0007 at the measuring box probe input port.

---

1. Select analog signal ( $\pm 1$  V,  $\pm 10$  V, 0...20 mA) at power cable 0554 0007.

Calling up the function:

>  → **Device settings** → **[OK]** → **Analog input** → **[OK]**.

#### Configuring the analog input:

1. **Measurement parameter** → **[Edit]**.
2. Enter or set values: **[▲]**, **[▼]**, **[◀]**, **[▶]** → **[OK]**.
3. Save the entry: **[Finished]**.
4. Entry of min. and max. measure value limit (**Min0V** or **Min0mA**) → **[Edit]**.
5. Enter or set values: **[▲]**, **[▼]**, **[◀]**, **[▶]** → **[OK]**.
6. **[Finished]**.

### 6.1.2.13. Data bus

#### Bus address

See Connection using a Data bus cable (accessory part to a bus system), page 36.

#### Bus rate

See Connection using a Data bus cable (accessory part to a bus system), page 36.

### 6.1.3. Fuels

The fuel can be selected. Fuel-specific coefficients (such as  $O_{2\text{ ref}}$ ,  $CO_{2\text{ max}}$  and  $SO_{2\text{ max}}$ ) can be set.

Besides the already pre-configured fuels, up to 5 more fuels can be configured in a customized way (e.g. with the **testo easyEmission** software). Fuel parameter, see [www.testo.com/download-center](http://www.testo.com/download-center) (registration required).



In order to maintain the measuring accuracy of the instrument one must choose or configure the correct fuel.

Calling up the function:

>  → **Fuels** → **[OK]**.

#### Activating fuels:

- > Select the fuel → **[OK]**.
- The fuel is activated and the main menu is opened.

### Setting coefficients:

1. Select the fuel → **[Coeff.]**.
2. Select the coefficients: **[Change]**.

Possibly:

- > Enter the password: **[Enter]** → **[Next]** → **[OK]**.
- 3. Set values → **[OK]**.
- 4. Save changes: **[Finished]**.

## 6.1.4. Sensor settings

An NO<sub>2</sub> addition and shut-down thresholds to protect the sensors can be set.

---



Recommended test gas concentrations and compositions can be found in the Testo Test Gas Manual (order no. 0980 2313 version D) or in the Download Centre.

---

Calling up the function:

- > **[Menu]** → **Sensor settings** → **[OK]**

### 6.1.4.1. NO<sub>2</sub> addition

The NO<sub>2</sub> addition value can be set.

The setting of the NO<sub>2</sub> addition value can be password protected, see Password protection, page 58.

Calling up the function:

- > **[Menu]** → **Sensor settings** → **[OK]** → **NO<sub>2</sub> addition** → **[Change]**.

Possibly:

- > Enter the password: **[Enter]** → Enter password → **[Next]** → **[OK]**.

### Setting the NO<sub>2</sub> addition:

- > Set parameter → **[OK]**.

### 6.1.4.2. CxHy-Sensor

The CxHy-Sensor can be activated / deactivated.

---



The **CxHy-Sensor** menu under **Sensor settings** is only displayed if an CxHy sensor is connected.

---

This sensor is a Pellistor which always requires a certain amount of O<sub>2</sub> to operate (approx. 2% O<sub>2</sub>). This sensor would be destroyed at lower values. The sensor therefore switches off at inadequate O<sub>2</sub> values. If it is known from the beginning that values below 2% do

exist, the sensor can also be switched off manually. CxHy-Sensor **On** starts the flue gas analyser with a zeroing phase (30s).

---

**i** For proper functioning the sensor is heated up to approx. 500°C, duration: approx. 10min. This means that the sensor needs to be zeroed again 10min after the device has been switched on, in order to prevent drifting (into the "minus" range).

---

Calling up the function:

>  → **Sensor settings** → **[OK]** → **HC-Sensor**

#### Switching the CxHy sensor on/off

1. **[Change]**.
2. Select setting: **[▲]**, **[▼]**
3. Confirm the entry: **[OK]**


### 6.1.4.3. Sensor protection

Protection limits can be set to protect the sensors against overload. The sensor protection switch-off is available for the following sensors: H<sub>2</sub>S, NO, NO<sub>2</sub>, CO<sub>2</sub>-(IR), CxHy, CO, SO<sub>2</sub>.

The sensor protection is activated if the threshold is exceeded, the measuring gas is diluted. If the threshold is exceeded again, the system will be shut down.

To deactivate sensor protection the thresholds must be set to 0ppm.

Calling up the function:

>  → **Sensor settings** → **[OK]** → **Sensor protection** → **[Change]**.

#### Setting sensor protection thresholds:

1. Select parameter: **[Edit]**
2. Set parameter → **[OK]**  
optional  
> Reset value to the factory setting: **[Default]**
3. Save changes: **[Finished]**

### 6.1.4.4. Calibration / adjustment

CO, SO<sub>2</sub>, NO<sub>2</sub>, NO, O<sub>2</sub>, H<sub>2</sub>S, CxHy and CO<sub>2</sub> (IR) sensors can be tested (calibrated) and adjusted using test gas.

Calibration/adjustment of the O<sub>2</sub> sensor (O<sub>2</sub> reference) is basically carried out in the same way as the calibration/adjustment of toxic sensors. The O<sub>2</sub> nominal value entered is only temporary, i.e. the nominal value will be overwritten with the ambient oxygen content

(21 Vol.%) the next time the instrument is switched off/on or when another zeroing process is carried out. The same applies when a measuring program passes through a zeroing phase. The O<sub>2</sub> test gas must also be applied to the measurement gas inlet (as with the toxic sensors).

---

**i** If obviously unrealistic readings are displayed, the sensors should be checked (calibrated) and, if required, adjusted. The calibration/adjustment can be carried out by the user or by a qualified service centre approved by Testo. To ensure that specific accuracies are retained, Testo recommends testing every six months and recalibration when required.

---

**i** Adjustments made with low gas concentrations can lead to accuracy deviations in the upper measuring ranges. The sensor protection (shut-down function) is not deactivated. The test gas concentration should therefore be lower than the set thresholds for the sensor protection. The function of **to dilute all** (x5) is automatically deactivated. If the instrument is fitted with an CxHy sensor, it should be switched off before test gas is applied.

---

**i** If a CxHy-Sensor is fitted, switch this off before measuring test gases with O<sub>2</sub> contents <2%. If you forget to do this, the sensor will switch off automatically during the measuring process, but will still be strained unnecessarily.

---

The following boundary conditions must be met when calibrating / adjusting:

- Use absorption-free hose material.
- Select **Testgas** as fuel
- Switch on the flue gas analyser at least 20 minutes before calibration / adjustment (to warm up)
- Use clean air for gas zeroing
- Maximum overpressure of the test gas 30hPa (recommended: pressureless via bypass)
- Apply the test gas for at least 3 minutes

Recommended test gas concentrations and compositions can be found in the Test Gas Manual (Order-No. 0981 2313) or in the Download Centre.

Calling up the function:

---

**i** Make sure that the ambient air is free of interfering gases (e.g. CO, NO, etc.) during zeroing!

---

- >  → **Sensor settings** → [OK] → **Calibration /Adjust** → [OK].

Possibly:

- > Enter the password: [Enter] → Enter password → [Next] → [OK].  
 - Gas zeroing (30s).

### Perform calibration / adjustment of CO<sub>2</sub>-, SO<sub>2</sub>-, NO<sub>2</sub>-, NO-, O<sub>2</sub>-, H<sub>2</sub>S-, CxHy-sensors:

#### **WARNING**

Dangerous gases

#### **Danger of poisoning!**

- > Observe safety regulations / accident prevention regulations when handling test gas.  
 > Use test gases in well ventilated rooms only.



Application of test gas via service adapter (0554 1205) is recommended, or apply test gas directly to the probe tip to avoid possible absorptions in the gas path.

1. Select the parameter: [▲], [▼] → [OK]
2. [Change] → Enter the test gas concentration (nominal value).
3. Apply test gas to the sensor.
4. Start calibration: [Start]
5. Once the actual value is stable, apply the nominal value (i.e. adjust the sensor to the nominal value) via [Adjust]. The values are stored in the record.  
 - or -  
 Carry out a comparison (calibration) between nominal and actual value via [Calibr.] without adjusting the sensor, and the values are stored in the record.  
 - or -  
 Cancel (no adjustment/calibration): [esc]
6. Save changes: [Finished]

### Perform calibration / adjustment of the CO<sub>2</sub>-(IR) sensor

Check the CO<sub>2</sub>-(IR)-sensor with the absorption filter to obtain accurate readings. The displayed CO<sub>2</sub>-value should be <0.03%CO<sub>2</sub>. If the value is higher, perform calibration and gradient adjustment.

### **WARNING**

Dangerous gases

#### **Danger of poisoning!**

- > Observe safety regulations / accident prevention regulations when handling test gas.
- > Use test gases in well ventilated rooms only.



Application of test gas via service adapter (0554 1205) is recommended, or apply test gas directly to the probe tip to avoid possible absorptions in the gas path.

1. Select the **CO<sub>2</sub>IR**-sensor: [**▲**], [**▼**] → [**OK**]
2. Connect Absorptionsfilter or apply Testgas CO<sub>2</sub> with 0%.
3. [**◀**], [**▶**], [**Yes**] → [**OK**]
  - Stability time (300s)
4. Start meas. val. admis. manually: [**Start**]  
or  
wait for stability time: Meas.val. admis. is automatically started.
  - Meas. val. admis. ends automatically.
5. [**Next**]
6. Enter the nominal gradient value: [**Change**] → [**▲**], [**▼**], [**◀**], [**▶**] → [**OK**].
7. Start stability time: [**Start**]
  - Stability time (300s)
8. Start meas. val. admis. manually: [**Start**]  
or  
wait for stability time: Meas.val. admis. is automatically started.
  - Meas. val. admis. ends automatically.
9. Perform adjustment: [**Finished**]  
-or-  
Cancel (no adjustment): [**esc**]


### 6.1.4.5. **ppmh counter**

The current ppm/h value can be displayed for the CO, COlow, NO, NOlow sensors.



The hour meter can be reset for the NO sensor, which uses a replaceable filter for neutralizing transverse gases.

Calling up the function:

- > [] → **Sensor settings** → [**OK**] → **ppmh counter** → [**OK**].
- The display shows maximum, current and remaining filter lifetime.

**Reset hour meter (NO sensor only)**

1. **[Reset]**.
2. Confirm confirmation request: **Yes** → **[OK]**

**6.1.4.6. Calibration data**

Use this function to display the current calibration data (comparison of nominal value and actual value without sensor adjustment).

Calling up the function:

- > **[Menu]** → **Sensor settings** → **[OK]** → **Calibration data** → **[OK]**.

Options

- > **[Options]** → **[Print]**: The current calibration data of all sensors are printed out.

**6.1.4.7. Adjustment data**

Use this function to display the current adjustment data and the sensor status of the individual sensors.

The condition of the sensor is checked every time the sensor is adjusted. The graph view shows the last 25 adjustments.

Call up function:

- > **[Menu]** → **Sensor settings** → **[OK]** → **Adjustment data** → **[OK]**

Options

- > **[Options]** → **[Print]**: the current adjustment data for all sensors is printed out.
- > **[Options]** → **[Graphic]**: the status of the selected sensor is graphically displayed.

Threshold	Explanation
100%	Full capacity
70%	Reduced sensor sensitivity. Recommendation: Acquire a replacement sensor
50%	Replace sensor

**6.1.4.8. Negative value**

The display for negative values can be activated / deactivated.

Calling up the function:

- > **[Menu]** → **Sensor settings** → **[OK]** → **Negative values**

**Switching negative values on/off**

1. **[Change]**
2. Select setting: **[▲], [▼]**
3. Confirm the entry: **[OK]**

**6.1.5. Programs**

Five flue gas measuring programs can be set, saved and executed. The **Trigger** function (trigger signal as start/stop criterion) is only available for devices with the trigger input option.

---

**i** Instrument settings cannot be changed if a program is active or running.

---

**i** The program **Flue Gas (before + after cat)** checks whether the meas. box is equipped with a fresh air valve. If not, a measuring program with normal flue gas measurement will be added, instead of the program **Flue Gas (before + after cat)**. A program **Flue Gas (before + after cat)** without fresh air valve does not show any sensible measuring results.

---

Calling up the function:

> **[Menu]** → **Programs** → **[OK]**.


**Activating / deactivating a program:**


- > Select the program: **[▲], [▼]** → **[Enable]** or **[Disable]**.
- When activating a program: The program is activated and the measurement type matching the program is opened.





**Editing the measuring program:**

Adjustable parameters:

Parameter	Function
Measurement program	Edit program name
Measurement type	Select flue gas menu: <ul style="list-style-type: none"> <li>• Flue gas</li> <li>• Flue gas + m/s</li> <li>• Flue gas ΔP</li> <li>• Flue gas (before and after catalyst)</li> <li>• Solid fuel</li> </ul>

Parameter	Function
Reading per mean value	<p>Mean value <b>Yes</b>: the measurement system saves one reading per second (measurement rate cannot be changed). At the end of the gas phase, a mean value is calculated from the individual values saved thus far and stored.</p> <p>Mean value <b>No</b>: when the end of the gas phase is reached, the values measured at this time are stored.</p>
Start	<p>Determine the start criterion</p> <ul style="list-style-type: none"> <li>•  The measuring program is started at any time (the function key automatically changes to the stop function).</li> <li>• Time Start of measurement at a pre-programmed time.</li> <li>• External signal Trigger signal to control the start of measuring programs.</li> <li>• Multi-point You can manually save multiple readings in a report while a measurement program is running, for example from different measuring points or from different load levels. In so doing, it is not possible to change the gas time, mean value, rinsing time and measurement rate. The load level or the firing rate for the individual measuring points can for instance be pre-selected in the display under <b>Options</b>.</li> </ul>

Parameter	Function
Stop	<p>Determining the stop criterion</p> <ul style="list-style-type: none"> <li>•  The measuring program is stopped at any time (the function key automatically changes to the start function)</li> <li>• Time The recoding of readings stops at a desired time.</li> <li>• External signal Trigger signal to control the stop of measuring programs.</li> <li>• Duration Setting cycles to save readings.</li> <li>• Memory full Saving readings ends when the memory is full.</li> </ul>
Gas time	Selection of gas time cycle
Rinse time	<p>Enter the rinse time (see <b>Recommendation for emission measurements over an extended period of time</b>, page 102).</p> <hr/> <p><b>i</b> The measurement program always begins with a rinse phase (duration: 30 sec). Measuring phases (gas time) and rinsing phases (rinsing time) alternate according to the programmed values.</p>
Meas. rate	The meas. rate is the saving cycle for mean values It is programmed in units of seconds, minutes, whereby the smallest possible meas. rate depends on the number and type of connected probes.

1. Select the program: ,  → [OK].
2. Press [Change].
3. Press [Change].
4. Edit program name: , , [, [].
5. Confirm the entry: [OK].
6. Repeat steps 4 and 5 as required.
7. Press [Next].

8. Perform steps 4 and 7 for further criteria accordingly.
9. Press **[Finished]**.

## 6.2. Measuring

### 6.2.1. Preparing for measurement

---

**i** If no combustion air temperature (AT) probe is connected, the temperature measured by the thermocouple of the flue gas probe, or the external thermocouple connected to the probe socket during the zeroing phase, is used as the combustion air temperature.

---

#### Note

Neither the flue gas probe nor the external thermocouple must be inserted into the flue gas duct during the zeroing phase.

---

All dependent parameters are calculated using this value. This method of measuring combustion air temperature is sufficient for systems dependent on ambient air. However, ensure that the flue gas probe is near the intake duct of the burner during the zeroing phase! If a combustion air temperature probe is connected, the combustion air temperature is measured continuously via this probe.

Following the zeroing phase, the currently measured temperature is displayed as the flue gas temperature (FT).

---

**i** The combustion air temperature (VT) is continuously measured by the temperature sensor installed in the meas. box. The fresh air required for the zeroing phase is drawn in through the exhaust if no fresh air valve (option) is installed and through the valve inlet if a fresh air valve is installed. The flue gas probe can thus already be inside the flue gas channel before or during the zeroing phase.

Exception: when using an analyzer unit with no fresh air valve and overpressure in the flue gas duct, the flue gas probe must be removed from the flue gas duct for zeroing.

---

**i** The testo 350 can be operated as follows:

- lying down
- hanging horizontally down by its handle
- plugged vertically to the wall bracket by the handle

To prevent measuring errors the position of the testo 350 must not be changed during a measurement.

---

---

**i** Under ambient temperatures of  $<10^{\circ}\text{C}$  the  $\text{CO}_2$ -(IR) sensor requires a shorter heat-up time to reach full measuring accuracy. At  $-5^{\circ}\text{C}$  this typically is 15min.

---

### **Before switching on**

- > Check whether:
  - All system components are properly connected.
  - All required probes / sensors are connected.
  - The power supply of all system components is guaranteed.

### **During then zeroing phase**

During the zeroing phase the sensors of the flue gas analyser are zeroed. Zero point and drift of the sensors are checked. The  $\text{O}_2$  value is set to 21%  $\text{O}_2$ .

- > Make sure that the ambient air is free of interfering gases (e.g.  $\text{CO}$ ,  $\text{NO}$ ) during the zeroing phase!

### **Before the measurement**

- > Set the fuel for the furnace system to be measured.
- > Assign the required measurement parameters and units to a display field in the measurement view.
- > Activate the location to which the readings are to be assigned.
- > Make sure that the gas outlets are free, so that the gas can escape without obstruction. Otherwise the measurement results may be corrupted.

### **Measurements with the $\text{CxHy}$ sensor**

#### **WARNING**

Dangerous mixture of gases

#### **Danger of explosions.**

- > Perform measurements only in flue gas ducts.
- > Only measure gases which do not form a combustible mixture in the ambient air.

---

**i** There must always be sufficient oxygen in the flue gas to prevent the  $\text{CxHy}$  sensor from being destroyed. With an  $\text{O}_2$  content of less than 2% the  $\text{CxHy}$  sensor switches off automatically (protective function). Higher concentrations of silicones,  $\text{H}_2\text{S}$  and sulphurous hydrocarbons can also lead to the destruction of the  $\text{CxHy}$  sensor.

---

Zeroing takes place automatically when the CxHy sensor is activated. To ensure that accurate CxHy readings are obtained, you should then wait about 10min (with the instrument switched on) before starting another zeroing process manually.

To prevent the CxHy sensor from drifting during lengthy measurement operations, zeroing should be carried out from time to time.

## 6.2.2. Using the flue gas probe

### Removing plastic cap

> Before starting a measurement, remove the plastic cap fitted on the flue gas probe and set it aside. The plastic cap is required for the gas path check (see Section 5.5.2).

### Checking the thermocouple

> Make sure that the thermocouple of the flue gas probe does not touch the probe basket. Bend the thermocouple back if necessary.

### Aligning the flue gas probe

- > Turn the probe to align the thermocouple so that it is freely exposed to the flue gas flow.
- > Align the flue gas probe in the flue gas duct so that the tip is in the hot spot (area of the highest flue gas temperature).

## 6.2.3. Applications

You can choose from fixed saved and a user defined application (application defined on the basis of the measuring object).

The memory contains suitable device settings for the meas. box and typical fuels and calculations for these applications. These quickly provides you with optimized device configurations for the respective measuring task and the device will automatically inform you about important application specific peculiarities (information in the display).

### burner

- Fuels: **Natural gas, Coke oven gas, Town gas, Propane, Light oil, Diesel, Heavy oil, Briquette, Lignite, Wood Pellets, Coke, Bois, Wood 30%M, Bark 45%H, Bark 60%H, G20, G25, G30, Test Gas**
- Available measuring programs: **Flue Gas, Flue Gas + m/s, Flue Gas +  $\Delta P$ , Program for all analyzer boxes**

### turbine

- Fuels: **Natural gas, Coke oven gas, Town gas, Propane, Light oil, Diesel, G20, G25, G30, Test Gas**
- Available measuring programs: **Flue Gas, Flue Gas + m/s, Flue Gas +  $\Delta p$ , Flue gas before + after catalyst, Program for all analyzer boxes**

### Engine $\lambda > 1$ and engine $\lambda < 1$

- Fuels: **Natural gas, Coke oven gas, Town gas, Propane, Light oil, Diesel, Heavy oil, G20, G25, G30, Test Gas**
- Available measuring programs: **Flue Gas, Flue Gas + m/s, Flue Gas +  $\Delta p$ , Program for all analyzer boxes, Flue Gas before + after catalyst**
- Measurement program **Flue gas before + after catalyst**: Two analyzer units are required. For this measurement type, both analyzer units must have a fresh air valve.  
If one of the two meas. boxes is equipped with a measurement range extension (individual dilution), the test 350 will automatically recommend this meas. box to be used for **Before cat**.  
If the meas. box used for measurement **Before cat** is not equipped with the option measurement range extension, the device will recommend to install this option.  
If the meas. box used for the measurement **Before cat** is equipped with the dilution option and the CO sensor is plugged into the dilution slot, 5x will automatically be used for dilution. If a higher dilution factor has already been activated, this setting will be maintained.  
If the meas. box used for the measurement **Before cat** is equipped with the dilution option and the CO sensor is not plugged into the dilution slot, the device will recommend to replug the sensor accordingly.

### User-defined

- Fuels: **Natural gas, Coke oven gas, Town gas, Propane, Light oil, Diesel, Heavy oil, Briquette, Lignite, Wood Pellets, Coke, Bois, Wood 30%M, Bark 45%H, Bark 60%H, G20, G25, G30, Test Gas**

Calling up the function:

1.  → **Applications** → **[OK]**.



Press the function key **Options** to open configuration menus.

2. Selecting an application: ,  → **[OK]**.

3. Selecting fuel: [, ] → [OK].

### 6.2.3.1. Flue Gas, Flue Gas + m/s, Flue Gas + $\Delta p$ , Program for all meas. boxes, Flue Gas before + after catalyst

The flue gas menus (**Measurement Type**) are the central measuring menus, which – in addition to the readings measured with this function – contain the readings of all measurements performed (if selected in the menu **Measurement view**). All readings can also be saved in or printed out from these menus.

The flue gas menus can always be selected, irrespective of the plugged in sensors.

Measuring functions of the flue gas menu:

- The measurement type **Flue Gas** can be used to perform a flue gas measurement.
- The measurement type **Program for all analyzer boxes** can be used for e.g. a bus system, in which several flue gas analysers are interconnected. A measuring program can thereby be defined and transferred to all meas. boxes.
- The measurement type **Flue Gas before + after cat** enables synchronous measuring of flue gas concentration before and after the catalyst. For this flue gas menu two measuring boxes are required, which are linked via the Test Data bus. The readings of both meas. boxes are displayed parallel in the display of the Control Unit to provide a quick overview over the condition of the catalyst.
- With measurement type **Flue Gas + m/s** a flue gas measurement can be performed in parallel to a flow measurement (+ volume / mass flow calculation) via a Pitot tube (the connecting cable for the thermocouple of the straight Pitot tube must thereby not be connected to the sensor socket of the instrument).
- The measurement type **Flue Gas +  $\Delta P$**  can be used to perform a flue gas measurement with parallel differential pressure measurement.

---

**i** After measurements with high concentrations and after longer measurements the instrument should be rinsed with fresh air, so that the sensors can be regenerated again.

---



**i** Flow measurement: Before the measurement make the location settings (Pitot tube factor and correction factor), see Folders / Locations, page 44.

Do not measure for longer than 5min, as the drift of the pressure sensor could have the effect that the readings are outside the tolerance limits.



---

Calling up the function:


✓ Application selected.

> Choose the measurement type: [, ] → [OK].

### Options

- > [Options] → **Save**: The readings are saved in a record.
- > [Options] → **Print**: The readings from a record are printed.
- > [Options] → **Fuels**: Select fuel
- > [Options] → **Dilution**: Select the dilution factor.
- > [Options] → **Measurement view**: (This function is not available during a measurement): The configure measurement view menu is opened.
- > [Options] → **Folders**: (This function is not available during a measurement): - The folder Folders/Locations is opened.
- > [Options] → **Programs**: The programs menu is opened.
- > [Options] → **Recalibrate**: (This function is not available during a measurement): The gas sensors are zeroed.
- > [Options] → **Number of lines**: Change the number of measuring values per display page.
- > [Options] → **Show Graphic**: The readings are displayed in form of a line graph.
- > [Options] → **Configure Graphic**: The measurement parameters to be represented (max. 4) can be displayed () or hidden ()
  - Possibly: Gas zeroing (30s).
- > Depressurize the pressure sensor and perform pressure zeroing.

Performing the measurement:

1. Start measurement: [].



Undiluted CO reading

If a separate measurement of CO undiluted has not yet been carried out, this value is calculated using the readings of the flue gas probe and is updated continuously.

If CO undiluted has already been measured separately, the value obtained is adopted.

---

- The readings are displayed.

2. End the measurement, record readings: [].

### 6.2.3.2. Draught-Measurement

**i** No flue gas probes with preliminary filter may be used for draught measurements.

- ✓ A flue gas probe must be connected.
- ✓ The pressure socket of the instrument must be free (depressurized, not closed).

**i** Do not measure for longer than 5 min, as the drift of the pressure sensor could have the effect that the readings are outside the tolerance limits.

**i** The **automatic pressure zeroing** (retrofit by Testo Service) automatically zeroes the pressure sensor at regular intervals (60s), to prevent the typical drift of the pressure sensor.

- > **[Options]** → **Save**: The readings are saved in a record.
- > **[Options]** → **Print**: The readings from a record are printed.
- > **[Options]** → **Measurement view**: (This function is not available during a measurement): The configure measurement view menu is opened.
- > **[Options]** → **Folders**: The folder **Folders** is opened.
- > **[Options]** → **Show Graphic**: The readings are displayed in form of a line graph.
- > **[Options]** → **Configure Graphic**: The measurement parameters to be represented (max. 4) can be displayed (🟢) or hidden (🔴).

Calling up the function:

- > **Measurement type** → **Draught-Measurement** → **[OK]**.

Performing the measurement:

1. Start measurement: **[▶]**
  - Draught zeroing (7s).
  - Rinse (approx. 10s).
2. Position the flue gas probe in the hot spot (area of the highest flue gas temperature). The display showing the maximum measured flue gas temperature (FT) helps when positioning the probe.
  - The reading is displayed.
3. Quit measurement **[■]**.
  - The reading is maintained.

### Options:

- > **[Options]** → **Save**: The readings are saved in a record.
- > **[Options]** → **Print**: The readings from a record are printed.
- > **[Options]** → **Show Graphic**: The readings are displayed in form of a line graph.
- > **[Options]** → **Configure Graphic**: The measurement parameters to be represented (max. 4) can be displayed (+) or hidden (x).

### 6.2.3.3. Smoke number/HCT

Calling up the function:

- > **Measurement Type** → **Smoke number/HCT** → **[OK]**.

Determine smoke pump no. / smoke nos. / oil derivative with the smoke pump and enter manually:



The function is only available if the chosen fuel is an oil.

---

1. Select parameter → **[Change]**.
2. Enter data or values → **[Next]** or **[OK]**.

### Enter the heat carrier temperature (HCT):

- > **Heat carrier** → **[Change]** → Enter value → **[OK]**.

### Options

- > **[Options]** → **Reset values**: The entered values are deleted.
- > **[Options]** → **Save**: The readings are saved in a record.
- > **[Options]** → **Print**: The readings from a record are printed.

### 6.2.3.4. Gas rating

The function **Gas rating** is only available if the activated fuel is a gas.

Calling up the function:

- > **Measurement Type** → **Gas rating** → **[OK]**.

- The measuring duration is displayed.

3. When the adjusted gas flow is reached: **[■]**.

- The calculated gas flow and the gas burner capacity (in kW) are displayed.

### Options:

- > **[Options]** → **Print**: The readings from a record are printed.
- > **[Options]** → **Save**: The readings are saved in a record.

- > **[Options]** → **Enter Gas Flow**: Set the gas flow value.
- > **[Options]** → **Change unit**: The unit for the gas flow can be changed (**m3 > l** or **l > m3**).

### 6.2.3.5. Oil flow rate

The function is only available if the chosen fuel is an oil.

Calling up the function:

- >  → **Measurement Options** → **[OK]** → **Oil Flow** → **[OK]**.

#### Performing the measurement:

1. Select the parameters **Oil Flow** (of the oil nozzle) and **Oil pressure** (no effect on calculation): **[▲]**, **[▼]** → **[Change]**.
2. Enter values. **[▲]**, **[▼]** and partly **[◀]**, **[▶]** → **[OK]**.
  - The calculated oil burner capacity (in kW) is displayed.

#### Options:

- > **[Options]** → **Print**: The readings from a record are printed.
- > **[Options]** → **Save**: The readings are saved in a record.
- > **[Options]** → **Change unit**: The unit for the oil flow can be changed (**kg/h > gal/h** or **gal/h > kg/h**).

## 6.3. Analog outputs

(only available via tab **Analog output box**)



The analog output box is displayed like the meas. box. The tab contains the databus number.

---



The analog output unit 0554 3149 (accessory) is suitable for the output of up to 6 measuring channels in the form of analog signals (4 to 20mA). The analog output unit is connected to the instrument via data bus, and the configuration can be carried out via the control unit.

### **Power supply**

Power is supplied to the analog output box via the measuring box. The LED of the analogue output unit lights green when the power supply is correct.


Each individual output channel is thereby assigned to a measuring channel, the range of the respective measurement channel is entered and then corresponds to the 4 to 20 mA output of the output box connected to this channel. If the measurement range is exceeded 21-22 mA is still output, depending on load. If the measurement range is fallen short of, the output will be up to 3.5 mA.

The current value is set to 3.5 mA as start value for a non-adjusted analog output box and for cases of faults.

## Connections

The channels are electrically isolated towards the Testo databus. However, the individual channels are not electrically isolated among each other.

When connecting you must make sure that there are no undesired ground loops!

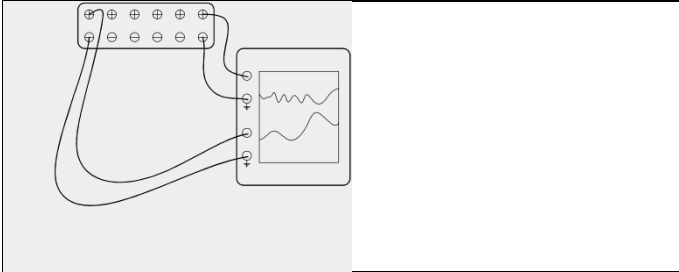

In both channels the positive output is connected to the ground connection of the recorder. The interfaces work correctly.

Calling up the function:

> [ ] → **Analog outputs** → [OK].

Configuration of analog outputs

1. Press [Edit].
  2. Assign channel to box: [▲], [▼] → [OK].
  3. Press [▶].
  4. Press [Edit].
  5. Select parameter: [▲], [▼] → [OK].
  6. Press [Edit].
  7. Set min. measurement limit: [▲], [▼], [◀], [▶] → [OK].
  8. Set max. measurement limit: [▲], [▼], [◀], [▶] → [OK].
  9. Select next channel: [▼].
- > Repeat steps 1 to 9.
10. Confirm the entry: [Finished].

## 7 Maintaining the product

### 7.1. Changing the rechargeable battery

#### Control Unit


---

**i** The rech. batt. pack can only be changed by the Testo service.

---

#### Meas. box

- ✓ The meas. box must not be connected to a mains socket.
- ✓ The meas. box must be switched off.

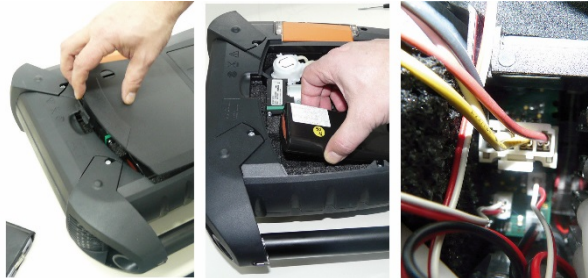

1. Open the cover of the service compartment (locking clip) on the back of the meas. box.
2. Take the rech. batt. pack out of the battery compartment and loosen the plug connection from the slot.

---

**i** Use only Testo rech. batt. pack 0515 5039. When inserting the rech. batt. pack, make sure that the leads do not get kinked or squeezed.

---

3. Connect the connector of the new rech. batt. pack to the slot and lay the rech. batt. pack into the battery compartment.
4. Close the service compartment cover.

### 7.2. Cleaning the flue gas analyser

- > In case of contamination clean the housings of Control Unit and meas. box with a damp cloth. Do not use any aggressive cleaning agents or solvents! Mild household cleaning agents and soap suds may be used.
- > Clean ventilation slots, gas outlets, fresh air inlets, pressure connections and dilution air inlet with a vacuum cleaner. Do not blow out with compressed air.

### 7.3. Changing / retrofitting sensors

---

**i** A slot bridge (0192 1552) must be inserted in slots which are not equipped with a sensor. Used sensors must be disposed of as hazardous waste!

---

**i** The CO<sub>2</sub>-(IR) sensor can only be changed / retrofitted by the Testo Service.

---

**i** CO H<sub>2</sub>-compensated sensors within the scope of the first German Federal Immission Control Ordinance (BImSchV) must only be changed / retrofitted by a Testo service centre.

---


**i** When retrofitting a sensor, the associated measurement parameter and unit must be enabled, see Section 6.1.4 Sensor settings.

---


**i** When changing the sensor, the current switch-off threshold values are only preserved if the analyzer unit is not disconnected from the rechargeable battery. If the switch-off thresholds need to be reset to the factory setting when changing the sensor, the analyzer unit must be disconnected from the mains and from the rechargeable battery.

---


- ✓ The latest instrument version must be installed on the measuring instrument (see Section 8.3 Updating the instrument software).
- ✓ The analyzer unit must be switched off and disconnected from the mains.
  1. Place the meas. box on its front.
  2. Open the cover of the sensor compartment (locking clip) and take it off.

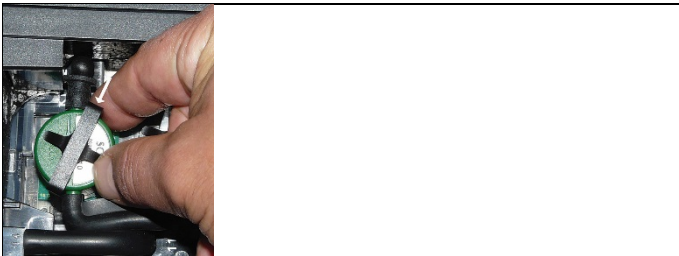

3. Loosen the bow from the sensor.

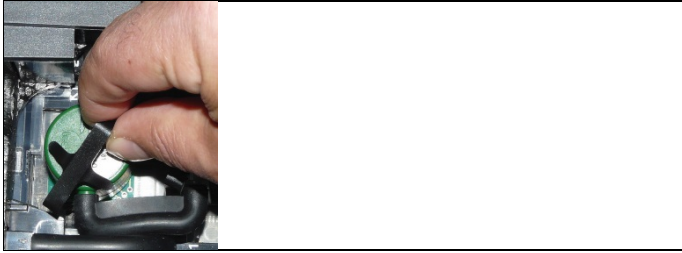

4. Take the sensor out of the bracket.
5. Pull the hose connections off the connecting nipples of the defective sensor / the bridge.
6. Remove the defective sensor /bridge from the slot.
  - > NO- / NO<sub>low</sub> sensors: Remove the auxiliary circuit board.

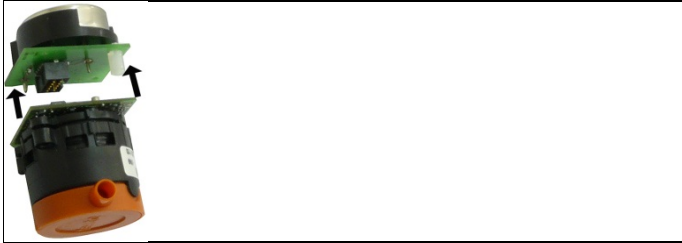


---

**i** Remove the additional circuit boards of the new sensors just before the installation. Do not allow sensors to lay around without additional circuit board for longer than 15min.


---

Sensors must be connected to the dedicated and correspondingly marked slots:

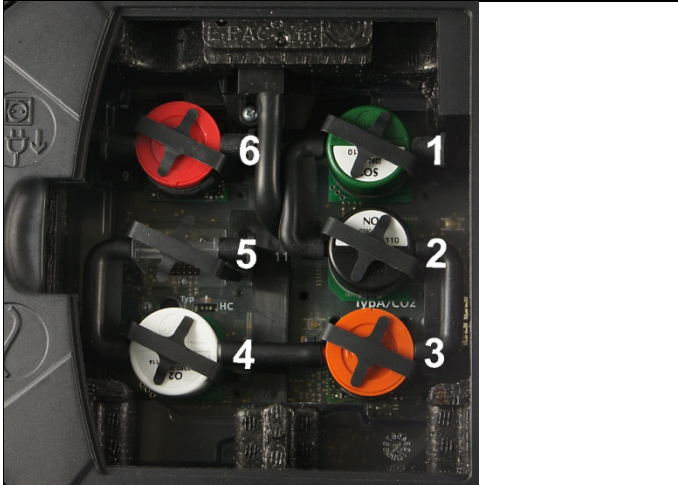

Slot	Sensors
1	NO <sub>2</sub> , H <sub>2</sub> S, CO, CO <sub>low</sub> , NO, NO <sub>low</sub> , SO <sub>2</sub>
2	NO <sub>2</sub> , H <sub>2</sub> S, CO, CO <sub>low</sub> , NO, NO <sub>low</sub> , SO <sub>2</sub>
3	CO <sub>2</sub> -(IR), NO <sub>2</sub> , H <sub>2</sub> S, CO, CO <sub>low</sub> , NO, NO <sub>low</sub> , SO <sub>2</sub>
4	O <sub>2</sub>
5	CO, CO <sub>low</sub> , NO, NO <sub>low</sub> , SO <sub>2</sub> , CxHy
6	CO, CO <sub>low</sub> , NO, NO <sub>low</sub> , SO <sub>2</sub> , CxHy

7. Install new sensor / new bridge in the slot.
8. Plug the hose connectors on the sensor / bridge.

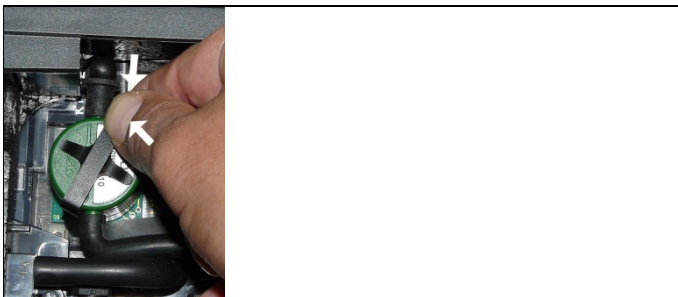

9. Insert the bow into the bracket.
10. Attach the sensor compartment cover and close it (the clip must click into place).


### 11. Switching on the analyzer box.

---

- i** After replacing an O<sub>2</sub> sensor, allow a 15-minute acclimatization time before using the instrument (establishing the supply voltage and initial stability time for new sensors).
- 

## 7.4. Replacing the filter for NO sensors

- ✓ The measuring instrument must be switched off and isolated from the mains supply.
1. Place the measuring instrument on its front.
  2. Open the cover of the sensor compartment (locking clip) and take it off.
  3. Loosen the bow from the sensor and take it out of the bracket, see Changing / retrofitting sensors, page 81.
  4. Pull the hose connectors off the sensor.
  5. Remove the sensor from the slot.
  6. Remove the used filter from the sensor.

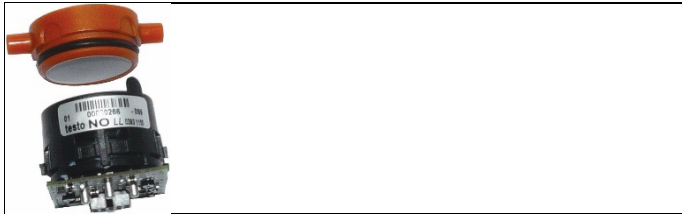

### 7. Plug the new filter on the sensor.

---

- i** Avoid touching the sensor. Follow the marking on filter and sensor.
- 

8. Insert the sensor in the slot.
9. Press the hose connectors on the sensor.
10. Insert the bow into the bracket, see Changing / retrofitting sensors, page 81.
11. Attach the service cover and close it (the clip must click into place).
12. Reset the ppm-hour meter, see ppmh counter, page 64.

## 7.5. Recalibrating sensors

See Calibration / adjustment, page 61..

## 7.6. Cleaning the modular flue gas probe

- ✓ Disconnect the flue gas probe from the measuring instrument prior to cleaning.
1. Release the probe catch by pressing the key on the probe handle and remove the probe module.



2. Blow compressed air through the flue gas ducts in probe module and probe handle (see illustration). Do not use a brush!
3. Fit a new probe module on the probe handle and engage it in place.

## 7.7. Replacing probe pre-filter


On probe modules with pre-filter the pre-filter can be replaced.

**i** Due to heavy dust loads, the probe preliminary filter should be checked regularly for contamination. Clean or replace the preliminary filter if the flow rate is too low (error message at a flow rate of  $< 0.6l$ ).

- > Unscrew the pre-filter from the probe shaft and screw on a new filter.

## 7.8. Changing the thermocouple

1. Release the probe catch by pressing the key on the probe handle and remove the probe module.

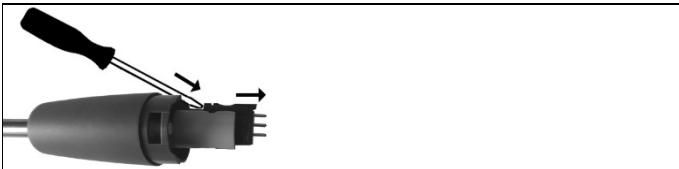

2. Remove the thermocouple plug-in head from the socket using a screwdriver and pull the thermocouple out of the probe shaft.
3. Keep inserting the new thermocouple into the probe shaft until the connection head clicks into place.

4. Fit a new probe module on the handle and engage in place.

### 7.9. Condensate trap / condensate container

With the gas preparation option fitted, the condensate is separated from the measuring gas and is led into a condensate container that is isolated from the gas path. In the case of longer measurements with moist flue gas, the condensate can be led off using a tube without any external air being carried along.

The filling level of the condensate trap can be read from the markings.

#### Emptying the condensate trap / condensate container

---

- i** The condensate consists of a weak mix of acids. Avoid skin contact. Make sure that the condensate does not run over the housing.
- 

#### **⚠ CAUTION**

Condensate entering the gas path.

#### **Damage to sensors and flue gas pump!**


- > Do not empty the condensate trap / condensate container while the flue gas pump is in operation.



1. Unlock the condensate trap / condensate container by the orange handle on the underside.



2. Unlock the condensate trap / condensate container and pull it vertically off the meas. box.

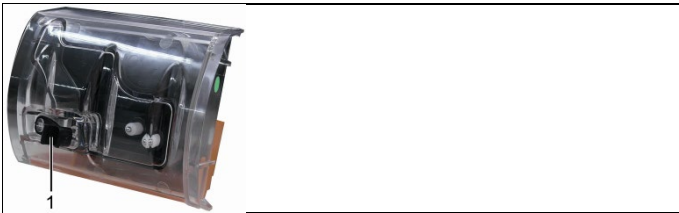

3. Open the drain plug (1) and let the condensate run out into a sink.
4. Wipe off any drops still on the condensate outlet with a cloth and close the condensate outlet.
5. Plug the condensate trap / condensate container on the meas. box.

## 7.10. Checking / replacing the dirt filter

### Checking the dirt filter:


- > Check the dirt filter of the meas. box periodically for contamination: Check visually by looking through the window of the filter chambers. In case of visible contamination: Change the dirt filter.

### Replacing the dirt filter:



The filter chamber may contain condensate.

---

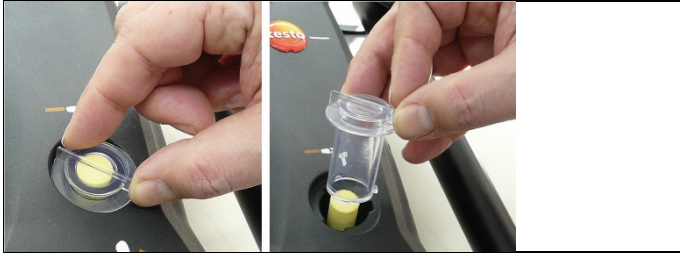

1. Open the filter chamber: Turn the filter cover anti-clockwise and take it off.




2. Remove the dirt filter and replace it with a new one 0554 3381).




3. Attach the filter cover and lock by turning it clockwise. The rib on the filter cover must be parallel to the handle.

### 7.11. **Cleaning / replacing the pump**

- ✓ The meas. box must be switched off and isolated from the mains supply.
1. Empty the condensate container.
  2. Place the meas. box on its front.

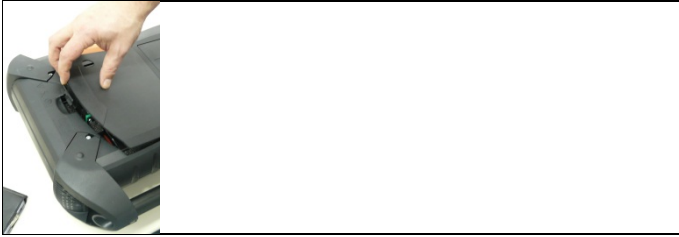

3. Open the cover of the service compartment (locking clip) on the back of the meas. box.

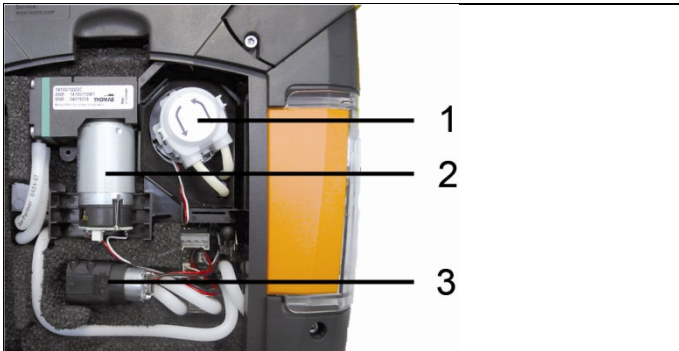

- 1 Condensate pump
- 2 Main gas pump
- 3 Rinsing / feed pump for diluting gas

### 7.11.1. Cleaning the main gas pump

1. Pull the gas pump upwards out of the gas measuring block.
2. Pull the inlet and outlet hoses off the sockets on the pump head
3. Loosen the plug connectors and remove the main gas pump.



4. Loosen the 4 fastening screws (Torx spanner T 9) on the pump head of the main gas pump.
5. Pull off the pump head.
6. Remove the two circlips from the depressions of the pump head (front and rear).
7. Remove and clean the pump diaphragm (e.g. white spirit).

- > If necessary, blow the inlet and outlet sockets out with compressed air.
- 8. Reattach the pump diaphragms with the circlips.
- 9. Place the pump head on the main gas pump and fasten with the screws (Torx spanner T 9).
- 10. Push the inlet and outlet hoses over the sockets on the pump head.
- 11. Connect the plug connectors and insert the main gas pump into the gas measurement block.

### 7.11.2. Changing the main gas pump

---

**i** When the main gas pump is changed by the user, the operating hour meter is not reset. The difference between the current operating hour reading and the operating hours from the last pump change serve as an indicator for the next pump change.

---


1. Pull the gas pump upwards out of the gas measuring block.
2. Pull the inlet and outlet hoses off the sockets on the pump head
3. Loosen the plug connector and remove the main gas pump.
4. Push the inlet and outlet hoses over the sockets on the pump head of the new main gas pump.
5. Connect the plug connectors and insert the main gas pump into the gas measurement block.

### 7.11.3. Changing the condensate pump


---

**i** The condensate pump is only available in instruments with the gas preparation (GP) option.

---

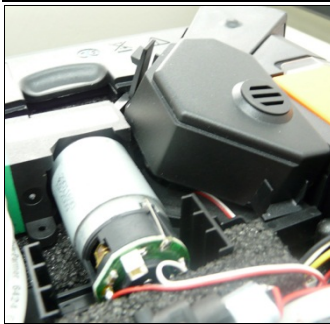


1. Unlock and remove the cover.

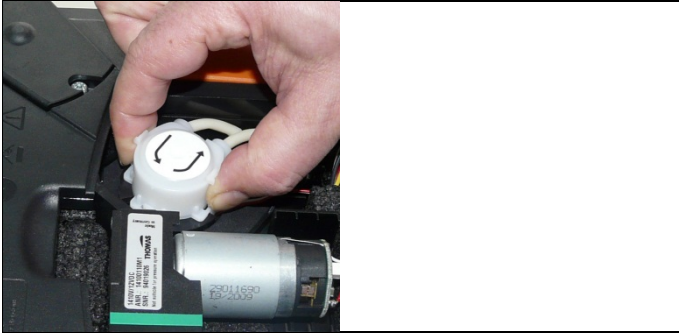


2. Unlock the two lateral clip locks of the condensate pump and pull off the pump head.
3. Pull the inlet and outlet hoses off the sockets on the meas. box.
4. Plug the inlet hose (length 25mm) and outlet hose (length 31mm) of the new pump onto the connecting sockets of the meas. box.
5. Push the pump onto the motor shaft until the clip locks engage. Make sure that the tubes are not pinched or constrained.
6. Attach cover.

#### 7.11.4. Replacing the motor of the condensate pump


**i** The condensate pump is only available in instruments with the gas preparation (GP) option.

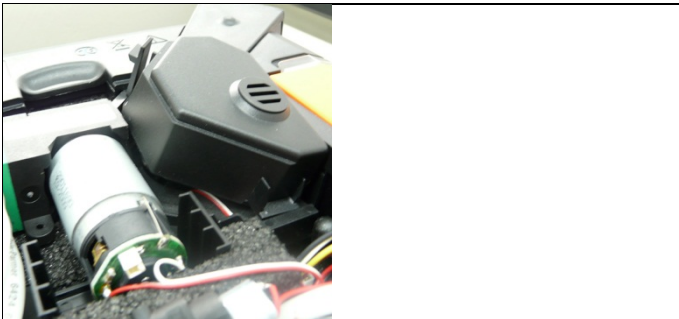


1. Unlock and remove the cover.

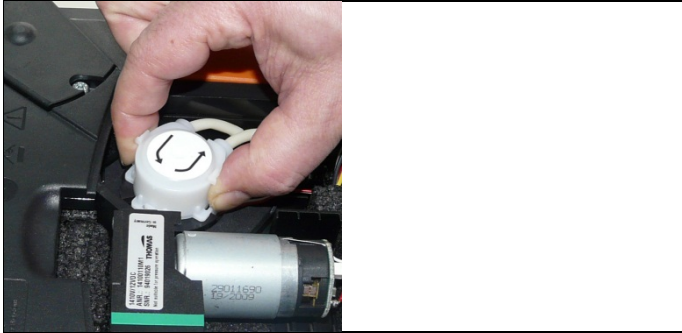

2. Unlock the two lateral clip locks of the condensate pump and pull off the pump head.
3. Pull the inlet and outlet hoses off the sockets on the meas. box.

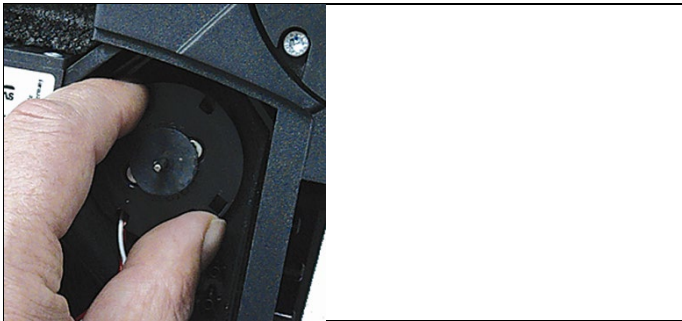

4. Loosen the motor on the condensate pump (short anti-clockwise turn).

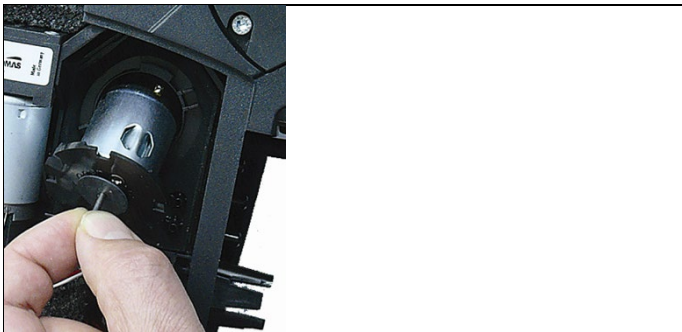

5. Take the motor of the condensate pump out of the bracket.
6. Loosen the plug connector, remove the motor.
7. Push on the plug connector of the new motor.

8. Place the motor of the condensate pump into the bracket.
9. Fasten the motor on the condensate pump (short clockwise turn).
10. Plug the inlet hose (length 25mm) and outlet hose (length 31mm) of the pump onto the connecting sockets of the meas. box.
11. Push the pump onto the motor shaft until the clip locks engage. Make sure that the hoses are not pinched or constrained.
12. Attach cover.


## 7.12. Replacing the filtration non-woven in the gas cooler

---


**i** The filtration non-woven is included in the filter set 0554 3381

---

- ✓ The meas. box must be switched off and isolated from the mains supply.
1. Unlock the condensate trap and pull it vertically off the measuring box.

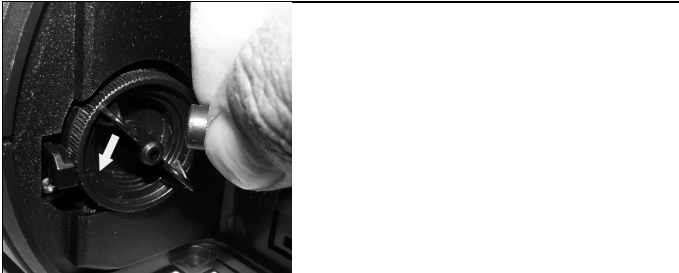

2. Pull off the hose.
3. Open the cover of the filtration non-woven in anti-clockwise direction.

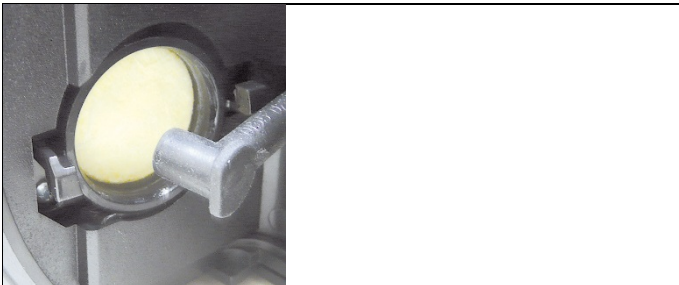

4. Replace the exhausted filter with a new filtration non-woven.
5. Close the cover.
6. Plug on the hose.
7. Plug the condensate container on the measuring box.

### 7.13. Recommended maintenance cycles

<b>Component</b>	<b>Service life</b>	<b>Remedy</b>
Main gas pump	2500h	Renew the pump
Special main gas pump for long-term measurement	10000h	Renew the pump
Rinsing/delivery pump	2500h	Renew the pump
Condensate pump	2500h	Renew pump head with hose
(gas cooler option)	5000h	Renew the pump
Fleece in gas cooler (gas cooler option)	1200h	Clean housing, renew fleece

## 8 Tips and assistance

### 8.1. Questions and answers

Question	Possible causes / solution
Rechargeable battery low	> Switch to mains operation.
Meas. box switches automatically off or meas. box cannot be switch on	Batteries / rechargeable batteries empty. > Charge rechargeable batteries or switch to mains operation.
NO value drifts	Auxiliary voltage for NO sensor was interrupted, e.g. by a sensor change. > Wait until sensor has regenerated. Stable NO measurement only possible after approx. 2h.
Double module	A sensor of the same type has already been plugged in.
Dilution	Gas flow rate in dilution path too high / too low > Please contact your local dealer or the Testo Customer Service.
O <sub>2</sub> sensor exhausted	> Replace the O <sub>2</sub> sensor
... Signal too high	Signal of indicated sensor is too high. > Wait until regenerated (additional zeroing starts automatically). > Ensure fresh air supply
... Signal not stable	Signal of indicated sensor is drifts excessively (defect). > Change sensor. > Wait until regenerated (additional zeroing starts automatically). > Ensure fresh air supply
... Switch-off	Reading of indicated sensor is higher than the set switch-off threshold.
Instrument temperature	Instrument temperature is beyond the operating temperature.
Pump volumetric flow rate	Too low gas flow (filter clogged) or too high gas flow (overpressure). > Check gas path / filter.

<b>Question</b>	<b>Possible causes / solution</b>
Gas cooling system	Gas cooler not working (faulty). > Please contact your local dealer or the Testo Customer Service.
Sensor temperature too high	O <sub>2</sub> sensor temperature beyond the specification.
Condensate in gas cooler was not pumped off.	Filter fleece is not absorbing condensate > Replace filter fleece, see Replacing the filtration non-woven in the gas cooler, page <b>93</b> . Condensate pump is not working > Check hose connections. > Replace condensate pump, see Changing the condensate pump, page <b>90</b> .
Low pump power	Inlet and outlet hoses mixed up by mistake. > Push the inlet and outlet hoses correctly over the sockets on the pump head.
Slow to establish a connection or slow data transfer between PC/notebook and testo 350 via Bluetooth	Control unit is plugged into measuring box or is connected via data bus cable. > To achieve a high data speed, we recommend setting up a Bluetooth connection directly via the measuring box.

If we could not answer your question, please contact your dealer or Testo Customer Service. Contact data see back of this document or website [www.testo.com/service-contact](http://www.testo.com/service-contact).

## 8.2. Accessories and spare parts

### Printer

<b>Description</b>	<b>Article no.</b>
test Infrared high-speed printer	0554 0549
testo Bluetooth® printer including rechargeable battery and mains unit	0554 0620

<b>Description</b>	<b>Article no.</b>
Spare thermal paper for printer, permanent ink	0554 0568

**Filter**

<b>Description</b>	<b>Article no.</b>
Particle filter for probe handle	0554 3385
20 pcs. dirt filters for measuring box	0554 3381
Replacement sintered filter for probe	0554 3372
Spare filter for NO-sensor	0554 4150

**Flue gas probes, probe shafts and thermocouples**

<b>Description</b>	<b>Article no.</b>
Flue gas probe, 335mm incl. probe stop, thermocouple NiCr-Ni (TI), Tmax 500 °C, 2.2m tube	0600 9766
Flue gas probe, 700mm incl. probe stop, thermocouple NiCr-Ni (TI), Tmax 500 °C, 2.2m tube	0600 9767
Flue gas probe, 335mm incl. probe stop, thermocouple NiCr-Ni (TI), Tmax 1000°C, 2.2m tube	0600 8764
Flue gas probe, 700mm incl. probe stop, thermocouple NiCr-Ni (TI), Tmax 1000°C, 2.2m tube	0600 8765
Flue gas probe, 335mm with pre-filter, incl. probe stop, thermocouple NiCr-Ni (TI), Tmax 1000°C, 2.2m tube	0600 8766
Flue gas probe, 700mm with pre-filter, incl. probe stop, thermocouple NiCr-Ni (TI), Tmax 1000°C, 2.2m tube	0600 8767
Engine probe with pre-filter, 335mm	0600 7555
Engine probe without pre-filter, 335mm	0600 7556
Tube extension 2.8m	0554 1202
Probe shaft with pre-filter, 335mm, Tmax 1000°C	on request
Probe shaft with pre-filter, 700mm, Tmax 1000°C	on request
Probe shaft, 700mm, Tmax 500°C TI	on request
Probe shaft, 335mm, Tmax 1000°C TI	0554 8764
Probe shaft, 700mm, Tmax 500°C TI	0554 8765

<b>Description</b>	<b>Article no.</b>
Thermocouple for engine probe, Tmax. +1000 °C and additional heat shield	0600 8898
Spare probe shaft, 335 mm, with pre-filter for flue gas probe for engine probe, Tmax 1000 °C	0554 7455

**Pitot tubes**

<b>Description</b>	<b>Article no.</b>
Pitot tube 350mm	0635 2145
Pitot tube 1000mm	0635 2345
Pitot tube 750mm, including temperature measurement and heat protection plate	0635 2042
Connection hose, silicone, length 5 m, maximum load capacity 700 hPa (mbar)	0554 0440

**Sensors (spare)**

<b>Description</b>	<b>Article no.</b>
O <sub>2</sub>	0393 0000
CO, H <sub>2</sub> -comp. filter cannot be changed	0393 0104
NO, filter not replaceable	0393 0150
NO <sub>2</sub>	0393 0200
SO <sub>2</sub>	0393 0250
SO <sub>2low</sub>	0393 0251
NO <sub>low</sub>	0393 0152
CO <sub>low</sub> -H <sub>2</sub> -comp.	0393 0102
CO <sub>2</sub> -(IR)	Testo-Sevice
H <sub>2</sub> S	0393 0350
CxHy	0393 0300

**Retrofits**

CO, H <sub>2</sub> -comp. sensor	0554 2104
NO sensor	0554 2150
NO <sub>2</sub> sensor	0554 2200
SO <sub>2</sub> sensor	0554 2250

NO <sub>low</sub> sensor	0554 2152
CO <sub>low</sub> -H <sub>2</sub> -comp. sensor	0554 2102
CO <sub>2</sub> -(IR) sensor	Testo-Sevice
H <sub>2</sub> S sensor	0554 2350
CxHy-sensor	0554 2300
Bluetooth® module for Control Unit and meas. box	Testo-Sevice
Gas cooler / gas preparation	Testo-Sevice
Fresh air valve	Testo-Sevice
Measurement range extension for individual slot	Testo-Sevice
DC voltage input	Testo-Sevice
Automatic pressure zeroing	Testo-Sevice

### Spare parts

Description	Article no.
Tube cartridge (condensate pump)	0440 0013
Motor for condensate pump	0238 0001
Rinsing / feed pump for diluting gas	0239 0014
Main pump (standard)	0239 0031
Special main gas pump for long-term measurement	0239 0032
Rech. batt. pack for meas. box	0515 5039
Rech. batt. pack for Control Unit	Testo-Sevice

### Other accessories

Description	Article no.
Service adapter	0440 1205
Mains unit for Control Unit	0554 1096
easy Emission (PC configuration software)	0554 3334
Transport case	0516 3510
Analog output box set	0554 3149
Cable with battery terminals and adapter for connection to meas. box	0554 1337
USB cable to connect the PC to the flue gas analyser	0449 0073

Description	Article no.
Data bus line 2m	0449 0075
Data bus line 5m	0449 0076
Other cable lengths up to 800 m	on request
ISO calibration certificate for flue gas	0520 0003

For a complete list of all accessories and spare parts, please refer to the product catalogues and brochures or look up our website [www.testo.com](http://www.testo.com)

### 8.3. Updating the instrument software

Under [www.testo.com/download-center](http://www.testo.com/download-center) you can download the current instrument software (Firmware) for testo 350 (registration required).

---

**i** Control Unit and meas. box must be separated for updating the instrument software.

---

**i** Before the firmware update is started, the control unit's rechargeable battery must be fully charged. If the battery is not fully charged, this will affect the firmware update. The flue gas analyser must then be sent in to Testo Service.

Once the instrument software has been updated, the descriptions in the operating instructions will no longer match the instrument functions. For the latest version of the operating instructions, visit [www.testo.com/download-center](http://www.testo.com/download-center).

---

#### Control unit

- > Unplug the mains unit and switch off the Control Unit.
- 1. Hold **[▲]** depressed.
- 2. Plug in the mains unit, keep **[▲]** depressed.
  - The display shows **Firmware update** along the bottom edge.
- 3. Release **[▲]**.
- 4. Plug the connecting cable (Art.-No. 0449 0073) into the USB-port on the Control Unit, then connect it to the PC.
  - Your PC recognises the Control Unit as a removable medium.
- 5. Copy the new file (appcurel.bin) to the detected removable medium.
  - In the display the status bar progresses from left to right. This process may take a few minutes.
- 6. Disconnect the connecting cable from the device.

- After updating of the instrument software (Firmware) has been completed the Control Unit will automatically reboot and is ready for use.

### Meas. box

> Disconnect mains plug

1. Place the meas. box on its front.
2. Open the cover of the sensor compartment (locking clip) and take it off.



3. Hold the button at slot 3 carefully depressed with a pointed tool.
4. Plug in the mains plug, keep the button depressed.
  - The status display flashes alternately green and red.
5. Release the button.
6. Plug the connecting cable (Art.-No. 0449 0073) into the USB-port on the meas. box, then connect it to the PC.
  - Your PC recognises the meas. box as a removable medium.
7. Copy the new file (appboxdbg.bin) to the detected removable medium.
  - The status display flashes alternately green and red. This process may take a few minutes.
8. Remove the connecting cable from the meas. box 350.
  - After updating of the instrument software (Firmware) has been completed the meas. box will automatically reboot and is ready for use.

## 9 Appendix

### Recommendation for emission measurements over an extended period of time

The following table shows recommendations for rinse times for measurements with high concentrations and recommendations for calibration cycles for emission measurements over an extended period (via a measuring program):

- > Rinse the instrument: Expose the probe to fresh air and start flue gas measurement.

Measurement parameter	Concentration [ppm]	Recommended measurement period [min]	Recommended rinse time [min]	Recommended calibration cycle in months	Filter service life
COH <sub>2</sub>	50	90	5	3	approx. 300.000ppmh
	100	60	5	3	
	200	30	10	3	
	500	15	10	3	
	1000	10	10	3	
	2000	10	15	3	
	4000	5	30	1	
	8000	5	45	1	
10000	5	60	1		
COH <sub>2low</sub>	10	90	5	3	approx. 80.000ppmh
	20	60	5	3	
	50	30	10	3	
	100	15	10	3	
	200	10	15	3	
500	10	20	3		
NO	50	90	5	3	approx. 120.000ppmh (filter exchangeable)
	100	60	5	3	
	200	30	5	3	
	500	20	10	3	
	1000	10	10	3	
	2000	10	20	1	
	3000	5	30	1	
	4000	5	30	1	

Measurement parameter	Concentration [ppm]	Recommended measurement period [min]	Recommended rinse time [min]	Recommended calibration cycle in months	Filter service life
NO <sub>low</sub>	10	90	5	3	approx. 40.000ppmh
	20	60	5	3	
	50	30	5	3	
	100	20	10	3	
	200	10	10	3	
	300	10	20	3	
NO <sub>2</sub>	10	90	5	3	-
	20	60	5	3	
	50	30	5	3	
	100	20	10	3	
	200	10	10	3	
	500	10	20	1	
SO <sub>2</sub>	50	90	5	3	approx. 200.000ppmh
	100	60	5	3	
	200	30	10	3	
	500	15	10	3	
	1000	10	10	3	
	2000	10	20	1	
	5000	5	40	1	
H <sub>2</sub> S	10	40	5	2	-
	20	30	5	2	
	50	20	10	2	
	100	10	10	2	
	200	5	10	2	
	300	5	20	2	
CxHy Pellistor	no rinsing cycles required, as long as the flue gas contains a sufficient amount of O <sub>2</sub> (O <sub>2</sub> shut-down...)			2	approx. 70.000ppmh
CO <sub>2</sub> -(IR)	no rinse cycles required			1	-



If the testo 350 is not used for measurements over an extended period, but rather, for example, for random measurements during start-up, servicing and adjustment of industrial combustion systems, process systems, power plants, gas turbines or stationary industrial motors, an

---

annual check of the testo 350 by Testo Service is recommended.

---

### Cross-sensitivities

This table is valid for new sensors with possibly unused filters, and for cross-gas concentrations in the ppm-range (down to less than 1000ppm).

The value "0" means: <1% cross-sensitivity.

Target gas	Cross-gas				
	CO	NO	SO <sub>2</sub>	NO <sub>2</sub>	H <sub>2</sub> S
O <sub>2</sub>	0	0	0 <sup>13</sup>	0	0
CO(H <sub>2</sub> )	---	0 <sup>10</sup>	0 <sup>10</sup>	0 <sup>10</sup>	0
CO(H <sub>2</sub> ) <sub>low</sub>	---	0 <sup>10</sup>	0 <sup>10</sup>	0 <sup>10</sup>	0
NO	0	---	0 <sup>10(w)</sup> <sup>11</sup>	6% <sup>12</sup>	0
NO <sub>low</sub>	0	---	0 <sup>10</sup>	<5% <sup>12</sup>	0
NO <sub>2</sub>	0	0	<-2%	---	-20% <sup>12</sup>
SO <sub>2</sub>	<5% <sup>12</sup>	0	---	-110% <sup>12</sup>	0 <sup>10</sup>
SO <sub>2</sub> <sub>low</sub>	<5% <sup>12</sup>	0	---	-110% <sup>12</sup>	0 <sup>10</sup>
CxHy	35% <sup>10</sup>	0 <sup>10</sup>	0 <sup>10</sup>	0 <sup>10</sup>	0
H <sub>2</sub> S	<2% <sup>12</sup>	<15% <sup>12</sup>	<20% <sup>12</sup>	-20% <sup>12</sup>	---

Target gas	Cross-gas				
	H <sub>2</sub>	Cl <sub>2</sub>	HCl	HCN	CO <sub>2</sub>
O <sub>2</sub>	0	0	0 <sup>13</sup>	0	see <sup>14</sup>

<sup>10</sup> With non-saturated filter.

<sup>11</sup> w = changeable filter

<sup>12</sup> Is compensated, if the cross-gas in the instrument is also measured (i.e. if the instrument is equipped with the corresponding sensors).

<sup>13</sup> No influence up to a few 1000ppm; for cross-concentrations in the %-range 0.3% O<sub>2</sub> per 1% SO<sub>2</sub> / HCl.

<sup>14</sup> 0.3% O<sub>2</sub> per 1% CO<sub>2</sub>; is compensated

Target gas	Cross-gas				
	H <sub>2</sub>	Cl <sub>2</sub>	HCl	HCN	CO <sub>2</sub>
CO(H <sub>2</sub> )	0 <sup>15</sup>	0	0	0	0
CO(H <sub>2</sub> ) <sub>low</sub>	0 <sup>15</sup>	0	0	0	0
NO	0	0	0	0	0
NO <sub>low</sub>	0	0	0	0	0
NO <sub>2</sub>	0	100%	0	0	0
SO <sub>2</sub>	<3%	-80%	0 <sup>10</sup>	30%	0
SO <sub>2,low</sub>	<3%	-80%	0 <sup>10</sup>	30%	0
CxHy	130% <sup>16</sup>	no data	no data	no data	0
H <sub>2</sub> S	0	<10%	0	0	0

---

<sup>15</sup> after H<sub>2</sub>-compensation

<sup>16</sup> Is compensated with indication H<sub>2</sub> from the CO(H<sub>2</sub>) sensor

